



Unstirred Water Baths

SBB Aqua Plus



EN

Operating Manual

Grant Instruments, based near Cambridge, England, is an independent, privately owned company, founded in 1951 by Peter Ward and Cecil Chapman.

Grant is a world leader in the manufacture and design of equipment for sample preparation, scientific analysis, data acquisition and data analysis providing solutions to the global scientific and industrial markets.

Standards Compliance and Quality

Grants' brand and reputation are based around quality, reliability and accuracy. We ensure our products stringently meet all necessary international safety standards.

We pay particular attention to the safety testing of products and remain at the forefront of the product safety standard for laboratory equipment IEC 61010-1. The company is committed to operating its safety test laboratory in accordance with the requirements of ISO 17025.

Grant operates a Quality Management System that complies with the requirements of BS EN ISO 9001:2008.

Beyond compliance to the standard, Grant is committed to continually improving in everything we do; with particular emphasis on understanding what matters to our customers and suppliers, and designing our systems and work to meet their needs.

If you have any feedback on Grant's products or services we would like to hear from you. Please send all feedback to:

Quality Manager
Grant Instruments (Cambridge) Ltd
Shepreth
Cambridgeshire
SG8 6GB
UK

Tel: +44 (0) 1763 260 811
Fax: +44 (0) 1763 262 410
E-mail: feedback@grantinstruments.com

Contents

1.0	Use of products	3
2.0	How to use this operating manual	3
3.0	Safety information	3
3.1	Safety compliance	3
3.2	Safety symbols	4
3.3	Safety warnings	4
4.0	Operating instructions	5
4.1	Unpacking instructions	5
4.2	Assembly of the equipment and components	5
4.3	Installation	5
4.4	Electrical supply	5
5.0	Operating procedures	6
5.1	Operation	6
5.1.1	Water level	6
5.1.2	Operation above 60°C	6
5.1.3	Flat bottomed vessels	6
5.1.4	Emptying the baths	6
5.2	Using the SBB Aqua Plus	7
5.3.1	Bath controls	7
5.2.2	Indicator lamps	7
5.2.3	Setting a controlled boil	7
5.2.4	Setting the constant level device	7
5.2.5	Resetting the over temperature cut-out devices	8
6.0	Technical specifications	8
7.0	Technical Tips	9
7.1	Which water should you use in your bath?	9
7.2	How to prevent rust in water baths	9
7.3	How to prevent algae and bacteria?	10
8.0	Warranty information	10
9.0	Maintenance and service	11
9.1	Cleaning	11
9.2	Fuses	11
9.2.1	Replacing fuses on SBB Aqua Plus	11
9.2.2	Routine safety tests	11
9.3	Service	12
10.0	Optional accessories	12
11.0	Troubleshooting	12
12.0	Contact Grant Instruments	13
13.0	Compliance	13

1.0 Use of products

The following products are covered by this operating manual:

- SBB Aqua (5, 12, 18 & 26) Plus

The products listed above are a general purpose series of thermostatically controlled unstirred water baths designed for indoor laboratory use by a professional user.

2.0 How to use this operating manual

This operating manual will allow you to unpack, set-up and operate this water bath correctly and safely. Important safety information, symbols and warnings are listed below and should be read carefully. Section 4 gives information about how to unpack and install the product correctly. Section 5 gives generic operating information in the first section followed by specific operating details for the SBB Aqua Plus baths respectively. Product technical specifications and tips are provided in the sections 6 and 7. The warranty for this water bath is detailed in section 8 but to register you should return the warranty card or complete the on-line registration form at www.grantinstruments.com.

If there is a technical matter that this operating manual does not address, or any other question concerning this product please contact Grant Instruments or your local distributor who will be able to provide any additional information.

3.0 Safety information

3.1 Safety compliance

Grant water baths meet the requirements of international safety standard IEC 61010: Safety requirements for electrical equipment for measurement, control, and laboratory use. They also comply with the equivalent national standards including:

EN 61010-2-010

UL 61010A-2-010

CAN/CSA-C22.2 NO. 61010-2-010-04.

3.2 Safety symbols

The symbols below are marked on the equipment to indicate:



Caution: Surfaces and water can be hot during and after use



Read this manual before using the bath



Important safety warning

3.3 Safety warnings



Read the whole of these instructions. Safety may be impaired if they are not followed.



If the equipment has been transported or stored in cold or humid conditions, condensation may form inside it. If that could have happened, allow time (at least 2 hours at room temperature) for the condensation to evaporate before using the equipment.



Do not use the bath to heat any material that could cause a fire or any other. Do not use the equipment in an area where there are aggressive or explosive chemical mixtures kind of hazard.



If a potentially hazardous liquid is spilt onto the equipment, disconnect it from the power supply and have it checked by a competent person. It is the user's responsibility to carry out appropriate decontamination if hazardous material is spilt on the equipment.



Before emptying a bath, allow the water temperature to fall to a safe level. For 18 and 26 litre baths, empty the bath before moving it.

The bath is for use only with water as the bath liquid. Make sure that it cannot become contaminated by other liquids. We recommend the use of de-ionised water.

Before first switching on the bath please remember to fill the bath with water. Switching the bath on dry will damage the heater and could invalidate the product warranty.

EN

4.0 Operating instructions

4.1 Unpacking instructions

Standard equipment includes:

- Thermostatic bath
- Mains cord with plug
- Gabled polycarbonate lid
- Metal base tray
- Operating manual

Remove packing materials carefully, and retain them for future shipment or storage of the equipment.

4.2 Assembly of the equipment and components

The water bath has three main components, the bath, the lid and the base tray. The base tray fits into the bath with the feet downward so that it creates a gap between the bottom of the tank and the tray. The lid should only be lifted by the handle provided as other parts can become hot during use. It also has a vent/thermometer hole - this hole should not be sealed as pressure could build up inside the bath.

4.3 Installation

Place the water bath on a level, non-combustible surface. Ensure that the mains plug and the switch are easily accessible.

4.4 Electrical supply

Check that the supply voltage marked on the serial number label, and the type of mains plug, are correct for your mains supply outlet, which must have a ground connector.

To disconnect the equipment from the mains supply, remove the mains plug from the mains supply outlet.

5.0 Operating procedures

5.1 Operation

5.1.1 Water level

Ensure that the baths are used with the appropriate base tray and that the water always covers the tray. The maximum water level should not be higher than the swage line around the top of the bath or around 2.5cm from the top. These criteria apply both when there are no vessels in the bath and with the maximum contents.

Avoid letting the bath run dry. In the event this does happen, the safety cutout will trip and disconnect the heater. If this does happen, unplug the bath and have the cut-out reset by a competent person.

5.1.2 Operation above 60°C

The lid must be used above 60°C to maintain proper temperature control and to ensure that the water temperature reaches the set point

The lid will also prevent excessive evaporation that requires the bath to be filled more often and will save energy.

5.1.3 Flat bottomed vessels


Do not place flat-bottomed vessels or other objects directly on the bottom of the tank. Always use the base tray. This avoids possible damage to the heater mounted under the tank. The base tray also improves temperature control.

5.1.4 Emptying the baths

Before emptying any bath allow the water temperature to fall to a safe level and take reasonable precautions to prevent accidental spillage.

5.2 Using the SBB Aqua Plus

5.2.1 Bath controls

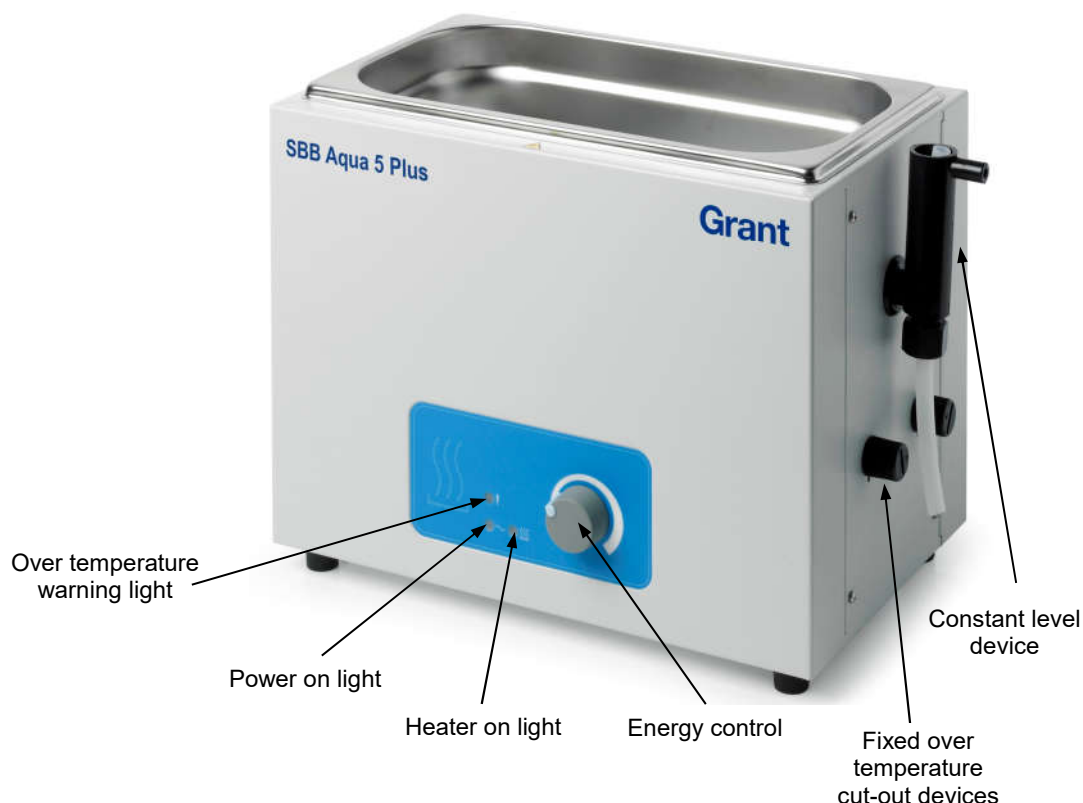

5.2.2 Indicator lamps

There are three indicator lights:

1. Power on (green).
2. Heater on (orange). Marked SSS .
3. Warning (orange). Marked $!$ indicates that one or both over temperature cut outs have tripped.

5.2.3 Setting a controlled boil

The bath can be set to boil continuously.

1. Turn the energy control knob to the maximum position.
2. When the water is boiling, reduce the power by turning the knob to a position that maintains the boiling at the desired level.

5.2.4 Setting the constant level device

A constant level device is fitted to the bath to maintain the required water level. To use the constant level device, connect the inlet pipe (black) to a water supply and the outlet pipe (white) to a drain. The water level can be adjusted by loosening the lower black nut and raising or lowering the white tube. The position of the top of the tube determines the water level. Re-tighten the black nut.

After filling the bath adjust the water flow rate to the minimum which maintains a constant water level when the water is boiling. Check that any relevant local water supply regulations are complied with if connecting to a mains water supply.

5.2.5 Resetting the over temperature cut-out devices

Two fixed over temperature cut-outs prevent the heater from overheating in the case of a low water level. The reset buttons for the over temperature cut-outs are on the side panel and can be reset by removing the protective black cap and pressing the red button in.

The over temperature cut-outs may activate during normal operation. If this is the case then they can be reset and the bath can continue to be used without compromising the safety of persons or the surroundings. However, if the cut-outs are persistently activated then it is recommended to have the bath checked by a competent person as soon as possible.

6.0 Technical specifications

Operating conditions

Ambient Temperature	5 to 40°C
Maximum relative humidity	80% R.H. in room temperatures up to 31°C decreasing linearly to 50 % R.H. at 40°C
Altitude above sea level	Up to 2,000 m (6,500 ft)
Operating Environment	Indoor use only

Electrical details

Mains supply: 230V @ 50/60 Hz or 120V @ 50/60 Hz

Pollution degree: 2

Installation Category: II

Note: Mains supply voltage fluctuations are not to exceed $\pm 10\%$ of the nominal supply voltage

Models	Capacity (L)	Current Rating (A)	
		120V	230V
SBB Aqua 5 Plus	5	11	6
SBB Aqua 12 Plus	12	11	7
SBB Aqua 18 Plus	18	11	9
SBB Aqua 26 Plus	26	11	9

SBB Aqua Plus bath performance

Temperature range	100°C only
-------------------	------------

7.0 Technical Tips

7.1 Which water should you use in your bath?

For the long-term reliability of water baths it is important to use oxygenated water that is free from ions and minerals that can cause corrosion of stainless steel. We recommend the use of distilled water and de-ionised water from modern ion exchange systems that do not use salt back flushing to regenerate the ion-exchange cartridges.

Stainless steel is protected from corrosion by a layer of chromium oxide. If the layer is damaged, oxygen present in water can reform the oxide layer. If the water is still or de-oxygenated, and the oxide layer is damaged, ions can corrode the stainless steel tank. If a water bath has been unused for some time, or water boiled, we recommend changing to fresh distilled water or correct de-ionised water.

Water normally contains calcium or magnesium ions. De-ionised water has most ions removed as indicated by its conductivity level; the purer the water the lower the conductivity. It is important to use only de-ionised water from an ion exchange system with replaceable cartridges. Do not use de-ionised water generated from an ion-exchange system that incorporates a salt back-flush system to regenerate the ion-exchange resin as this can leave sodium ions that are very corrosive to stainless steel.

7.2 How to prevent rust in water baths

Most Grant tanks, as well as immersed parts, are made from type 304 stainless steel, an extremely versatile general purpose grade of stainless steel. It is the excellent forming characteristic that has made this grade dominant in the manufacture of laboratory and industrial water baths, as well as domestic sinks and saucepans. Type 304 stainless steel is highly suitable for applications where hygiene is important; it exhibits good heat resistance and excellent resistance to corrosion.

However, despite resistance to general surface corrosion, stainless steel is susceptible to specific types of corrosion, in particular pitting (small pin hole style corrosion) and stress corrosion cracking. It can also undergo general corrosion in specific environments, such as one containing hydrochloric or sulphuric acids.

Stainless steel is protected by its high content of alloying elements, primarily chromium and nickel. Chromium is the most important with respect to corrosion resistance, although the nickel assists in allowing the chromium to do its job. The chromium forms an oxide layer on the surface of the steel, which inhibits further oxidation. This layer adheres extremely well to the metal substrate, but it is essential that it remains intact, and must be protected from various forms of damage.

If the surface chromium oxide layer becomes damaged, oxygen present in water can partially reform the oxide layer, so it is advisable to ensure that water is always fresh and well oxygenated. Baths that will be out of use for an extended period should be emptied, and all moisture should be wiped from the bottom of the tank.

In some cases a brown layer may appear on the surface of a stainless steel tank. In most of these cases this is not rust, but it may be a surface deposit of minerals from the local water supply, or ferrous particles or salts that have fallen into the tank. These surface deposits can usually be removed by using a household cleaner such as Duraglit or Silvo metal polish.

7.3 How to prevent algae and bacteria?

Water baths provide the ideal environment for the growth of micro-organisms. If left uncontrolled the growth of these organisms can result in a range of serious problems and health risks from pathogenic bacteria.

The growth of algae on the surface of parts will cause biofouling which can reduce performance.

Micro-organisms that produce acidic metabolic by-products can cause bio-corrosion by depolarisation of metal surfaces.

There are a number of biocides available on the market.

8.0 Warranty information

When used in laboratory conditions according to this manual, this product is guaranteed for THREE YEARS against faulty materials or workmanship.

Extended warranty for years four and five can be purchased by contacting our sales department at salesdesk@grantinstruments.com.

9.0 Maintenance and service

No routine maintenance is required except for cleaning. There are no user serviceable parts inside the unit.

9.1 Cleaning

Clean the outside of the equipment with a damp cloth, using water only. Do not use chemical cleaning agents. Before using any other cleaning or decontamination method, check with Grant Instruments or your local representative to make sure that the proposed method will not damage the equipment. Scale on immersed parts can be removed using chemical de-scaling products designed for use on kitchen equipment that have metal parts. De-scaling products may be toxic and manufacturer's instructions should always be followed.

9.2 Fuses

Fuses are Littelfuse 3AB 314 series, fast-acting, high breaking current (max breaking current at least 750 A); dimensions are 1.25 inch long, 0.25 inch diameter. Replace fuses only by the same type and rating (250V).

Models	Fuse Rating (A)	
	120V	230V
SBB Aqua 5 Plus	15	15
SBB Aqua 12 Plus	15	15
SBB Aqua 18 Plus	15	15
SBB Aqua 26 Plus	15	15

9.2.1 Replacing fuses on SBB Aqua Plus

Disconnect the unit from the power supply

1. Remove the mains lead from the socket at the back of the bath.
2. Carefully use a screwdriver to unscrew the fuse cap from the holder. Check the fuse(s) and replace if necessary using the specified fuse type and rating. **CAUTION:** the fuse should be placed in the cap, do not attempt to put the fuse directly in the holder.
3. Carefully replace the fuse cap in the holder and replace the mains lead.

9.2.2 Routine safety tests

If routine tests are to be made, we recommend a test of the integrity of the protective earth conductor and an insulation test at 500 V DC. Routine flash tests are **not** recommended for any electrical equipment, because repeated high voltage tests degrade insulation materials.

9.3 Service

If service is required, switch off the unit and contact Grant Instruments or your local representative for repairs.

Service Department
Grant Instruments (Cambridge) Ltd
Shepreth
Cambridgeshire
SG8 6GB
UK

Tel: +44 (0) 1763 260 811
Fax: +44 (0) 1763 262 410
E-mail: labservice@grantinstruments.com

10.0 Optional accessories

A full listing of product accessories and options is available in the Grant Scientific Reference Catalogue (a copy of which is available upon request) and on the Grant website at www.grantinstruments.com.

11.0 Troubleshooting

No power on light - check power source, mains switch and fuses.

Water is not reaching temperature – increase energy input.

'Heater on' light will not come on. Check the over-temperature cut outs are set correctly. See Section 5.2.5 if these are already correctly set, then contact Grant Instruments.

'Over-temperature' warning light is lit. one or both of the over-temperature cutout has tripped. Reset the trips see Section 5.2.5.

12.0 Contact Grant Instruments

At Grant we are continuously trying to improve the performance we offer our customers. If you have any feedback on Grant's products or services we would like to hear from you. Please send all feedback to:

Quality Manager
Grant Instruments (Cambridge) Ltd
Shepreth
Cambridgeshire
SG8 6GB
UK

Tel: +44 (0) 1763 260 811
Fax: +44 (0) 1763 262 410
E-mail: feedback@grantinstruments.com

13.0 Compliance

WEEE directive

Grant Instruments complies fully with the Waste Electrical & Electronic Equipment (WEEE) regulations 2006. We are a member of the B2B compliance scheme (Scheme Approval Number WEE/MP3338PT/SCH), which handle our WEEE obligations on our behalf. Grant Instruments have been issued with a unique registration number by the Environmental Agency, this reference number is WEE/GA0048TZ.

For information regarding WEEE collections in the UK please contact our B2B Compliance Scheme directly on 01691 676 124.
For other countries please contact your equipment supplier.

For General WEEE information please visit: www.b2bcompliance.org.uk

RoHS directive

All the products covered by this manual comply with the requirements of the RoHS Directive (Directive 2011/65/EC).

Electrical safety and electromagnetic compatibility

All the products covered by this manual comply with the requirements of the Low Voltage Directive (2014/35/EC) for electrical safety and the EMC directive (2014/30/EC) for electromagnetic compatibility.

Notes

EN