

Bright

Instruments

Stable | Efficient | Safe

Bright Cryostat

OTF7000/LS AND OTF7000/HS



Stable

Stable temperature

The cryochamber temperature is adjustable between 0~-35°C. Compressor adopts frequency conversion working mode, intelligent temperature control. When the glass door is open for more than 2 hours, the temperature fluctuation within 2°C.

Effective specimen cooling system(optional), adjustable temperature range -10°C~-50°C with low pressure cooling system and semiconductor refrigeration, faster temperature regulation and low failure rate.

Stable section quality

The precision cross roller guide rails provide a guarantee for section smoothness and accuracy.

Precise screw rod meets the 0.5μm sample injection requirements.

The five-phase high-resolution stepping motor has higher positioning accuracy and lower motor vibration.

The horizontal sampling slide is made of aviation aluminium, with ultra-high strength and corrosion resistant material.



High quality section



Stable temperature



system



Effective specimen cooling system




Efficient



Efficient operating system


7 inch touch screen, intuitive and easy to operate.

The joystick integrates coarse sampling, trimming and section switching, and section parameter adjustment for efficient operation.

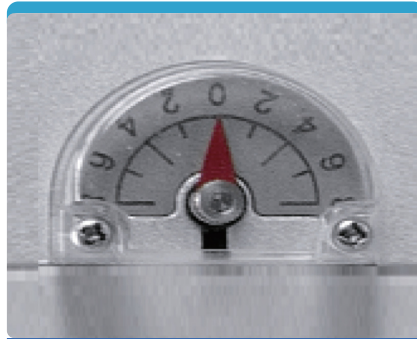

Rapid sample positioning

Precise positioning system with visual pointer, easy to adjust the sample to the target angle, reducing trimming and sample waste.

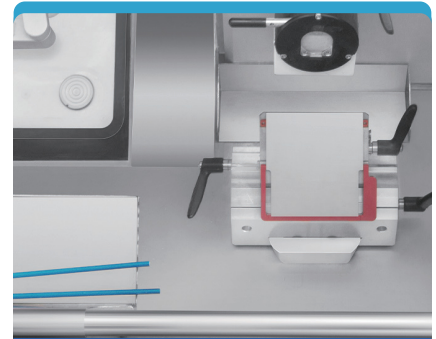

Efficient defrosting


Automatic defrosting for cryochamber, specimen head, quick-freeze shelf, more thorough.

For manual defrosting, there are different choices to improve efficiency.



Auto section

For extra ease of use and consistent sectioning of all specimen types, an optional auto section is available.

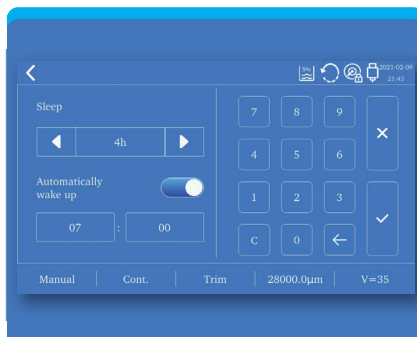

Auto sleep and wake up

Energy saving and environmental protection, meanwhile eliminate waiting time.



Specimen loading and marking

Single lever operation, efficient specimen loading. It provides maximum clamping force independent of individual user strength.

The unique label design of specimen discs makes it easy to record and identify each sample to prevent confusion.

Safe



UVC disinfection

For an extra measure of safety, the inside of the instrument features an UVC disinfection system, can be used at any time and low temperature. The intensity is above 340 uw/cm².



Ergonomic design


Ergonomic exterior cabinet with circular arc design.

The height adjustable footrest (optional) makes each user feel more comfortable.



Remove section waste

Section waste is easily removed by using the optional Section Waste Removal System, no need to clean by hand.

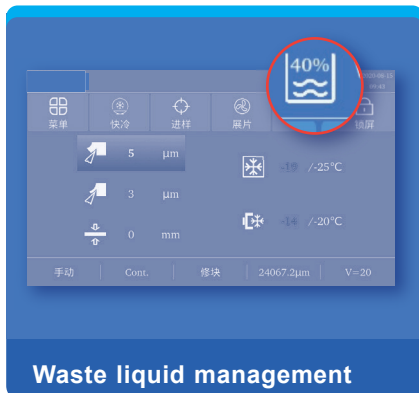

Waste liquid management

There is an icon show current storage. If it is above 90%, the icon will turn red. If the waste bottle is not in place, the icon will flash to remind.

Technical parameter

Section thickness range: 0.5 - 100 μm

0.5 - 5 μm in 0.5 μm increments

5 - 20 μm in 1 μm increments

20 - 30 μm in 2 μm increments

30 - 60 μm in 5 μm increments

60- 100 μm in 10 μm increments

Trimming section thickness range: 1 - 800 μm

1- 10 μm in 1 μm increments

10- 20 μm in 2 μm increments

20- 50 μm in 5 μm increments

50- 100 μm in 10 μm increments

100- 800 μm in 50 μm increments

Specimen retraction: 0-250 μm , adjustable

Horizontal feed: 28mm, vertical stroke: 70mm

Specimen orientation: 8°(X-, Y-axis), 360°rotation of specimen disc

Electric coarse feed: 0-1800 $\mu\text{m}/\text{s}$

Cryochamber temperature range: 0~-35°C

Specimen Cooling^(optional)temperature range: -10°C~-50°C

Quick-freeze shelf minimum temperature: down to -42°C, at chamber temp. -35°C

Number of freezing stations: 15

Peltier element temperature: reduced to -50°C~-60°C within 3 minutes, at chamber temp. -35°C

Number of freezing stations:2

Defrost: automatic defrost, manual defrost

UVC disinfection: 30 or 180 minutes , user selectable

Section mode: automatic section , manual section

Automatic section mode: Single, Cont., Int., Multi.

Electric section speed: 0.5~450mm/s

Width^(with handwheel) x Depth x Height: 860*865*1252mm

Working height(armrest): 1025mm

Customise on demand

You can choose different configurations and functions according to your research needs.

Model	Configuration	UVC disinfection	Vacuum	Specimen cooling system	Auto section	Note
OTF7000/LS	UV	√				For large specimen numbers and varying specimen types with UVCfor increased user safety.
	Specimen	√		√		Most popular cryostat with individually controlled temperature settings on both the cryochamber and the specimen holder.
	Vacuum	√	√	√		With vacuum cleaning system for optimized safety.
OTF7000/HS	Auto	√		√	√	With motorized section to improve reproducibility.
	Max	√	√	√	√	Fully automatic cryostat with vacuum cleaning system for whole function.



WolfLabs

Pricing on any accessories shown can be found by keying the part number into the search box on our website.

The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed to be correct. If there are aspects of the specification that must be guaranteed, please provide these to our sales team so that details can be confirmed.

www.wolflabs.co.uk

Tel : 01759 301142

Fax : 01759 301143

sales@wolflabs.co.uk

Please contact us if this literature doesn't answer all your questions.