

# CUBE digital dry baths

CUBE digital dry baths are available in single and dual block models, and have a comprehensive range of interchangeable blocks.

Each digital dry bath is compact and easy-to-use. The quick-change blocks have rapid heat-up times and reproducible temperature uniformity and accuracy, and may be used in a variety of applications, which include: restriction digestion, coagulation studies, hybridisation, Hot Start PCR® reactions and DNA denaturation. Due to the Solid Aluminium block holder, each Cube dry bath may also be adapted as a mini water bath incubator if desired. Both dry baths incorporate a digital microprocessor controller for accurate temperature control in 0.1°C increments from ambient +5°C to 150°C. Rapid and easy programming is facilitated by the easy to use arrow keys on the sloped front panel, while both the temperature and running time are shown simultaneously on the dual digital LCD display.




## KEY FEATURES

- Microprocessor control with digital performance for precise, accurate control
- Wide temperature control range with excellent uniformity
- Rapid temperature increase rate
- LCD screen showing timer and temperature simultaneously
- User temperature calibration

## TECHNICAL SPECIFICATIONS

Cat. No.	TCDB-01	TCDB-02
Number of blocks	1	2
Display	LCD Display	
Heating Power	125W	200W
Dimensions, mm (W x L x H)	15x15x13.5 mm	15x23x13.5 mm
Controller	Digital Microprocessor	
Heating Chamber	Molded aluminium alloy chamber	
Temperature Range	5°C above ambient to 150°C	
Temperature Increment	0.1°C	
Temp. Uniformity at 37°C	within 0.2°C	
Temp. Accuracy at 37°C	within 0.2°C	
Temp. Calibration	Yes	
Timer	Up to 99(hr) : 59(min), continuous	
Safety	Leak proof heating chamber Over temperature protection SSR failure detection	
Operating Temp.	Ambient to 40°C	

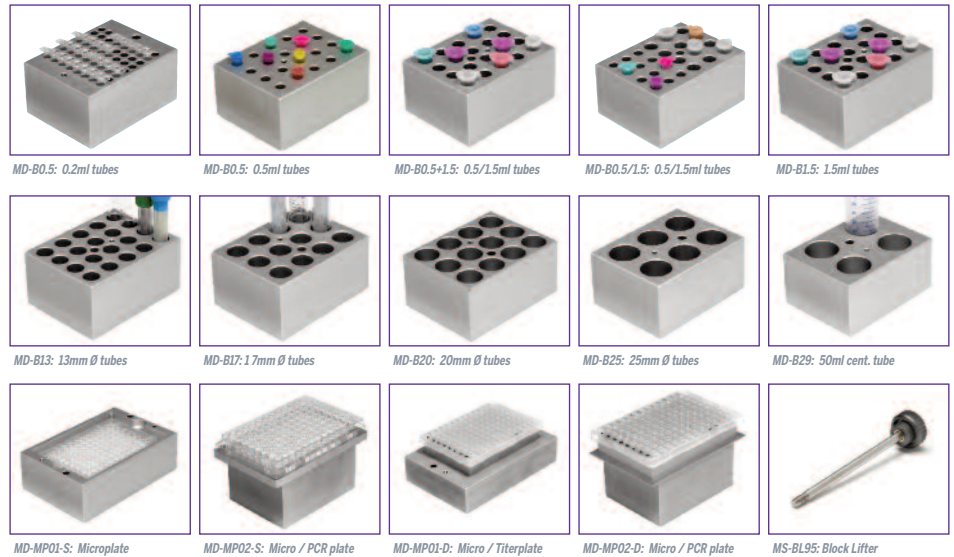

MD-B0.5: 0.2ml tubes

MD-B0.5: 0.5ml tubes

MD-B0.5+1.5: 0.5/1.5ml tubes

MD-B0.5/1.5: 0.5/1.5ml tubes

MD-B1.5: 1.5ml tubes

MD-B13: 13mm Ø tubes

MD-B17: 1.7mm Ø tubes

MD-B20: 20mm Ø tubes

MD-B25: 25mm Ø tubes

MD-B29: 50ml cent. tube

MD-MP01-S: Microplate

MD-MP02-S: Micro / PCR plate

MD-MP01-D: Micro / Titerplate

MD-MP02-D: Micro / PCR plate

MS-BL95: Block Lifter

## ORDERING INFORMATION

### SINGLE BLOCK

**TCDB-01\*** The Cube Dry Bath Incubator (one block unit); without block 220V

### DUAL BLOCK

**TCDB-02\*** The Cube Dry Bath Incubator (dual block unit); without block 220V

### Accessories

MD-MP01-S	Block for Microplate; Titerplate Plain Block for Single Block Unit Only
MD-MP02-S	Block for 96 wells deep Microplate or PCR plate for Single Block Unit Only
MD-MP01-D	Block for Microplate; Titerplate Plain Block for Dual Block Unit Only
MD-MP02-D	Block for 96 wells deep Microplate or PCR plate for Dual Block Unit Only
MD-B0.5/1.5	Double side block: one side for 1.5 or 2.0 ml tube, 20 wells; Opposite side for 0.5 ml tube, 30 wells
MD-B0.5PLUS1.5	Combination block : for 0.5 ml tube, 12 wells and for 1.5 or 2.0 ml tube, 12 wells (on the same side)
MD-B0.2	Block for 0.2 ml tube, 64 wells or for 0.2 ml PCR strip tubes for 8 wells x 8

MD-B0.5	Block for 0.5 ml tube, 20 wells
MD-B1.5	Block for 1.5 ml tube, 20 wells
MD-B13	Block well size 13 mm, 20 wells
MD-B17	Block for 15 ml centrifuge tube, 12 wells
MD-B20	Block well size 20 mm, 12 wells
MD-B25	Block well size 25 mm, 6 wells
MD-B29	Block for 50 ml centrifuge tube, 4 wells

\* For 110V units, add \$ to order code



**Wolflabs**

# Wolf Laboratories Limited

[www.wolflabs.co.uk](http://www.wolflabs.co.uk)

Tel: 01759 301142

Fax: 01759 301143

[sales@wolflabs.co.uk](mailto:sales@wolflabs.co.uk)



**Use the above details to contact us if this literature doesn't answer all your questions.**

**Pricing on any accessories shown can be found by keying the part number into the search box on our website.**

The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed to be correct. If there are aspects of the specification that must be guaranteed, please provide these to our sales team so that details can be confirmed.

