

Safety

Please read this information carefully prior to installing or using this equipment.

1. The unit described in this manual is designed to be operated only by trained personnel. Any adjustments, maintenance and repair must be carried out as defined in this manual, by a person qualified to be aware of the hazards involved.
2. It is essential that both operating and service personnel employ a safe system of work, in addition to the detailed instructions specified in this manual.
3. Other than for those items defined in the maintenance procedures herein there are no user serviceable items in this instrument. Removal of covers and attempted adjustment or service by unqualified personnel will invalidate the warranty and may incur additional charges for repair.
4. References should always be made to the Health and Safety data supplied with any chemicals used. Generally accepted laboratory procedures for safe handling of chemicals should be employed.
5. If it is suspected that safety protection has been impaired in any way, the unit must be made inoperative and secured against any intended operation. The fault condition should immediately be reported to the appropriate servicing authority.

Merci de lire attentivement ces informations avant d'installer ou d'utiliser cet appareil.

1. L'appareil décrit dans ce manuel est conçu pour être utilisé uniquement par des personnes formées. Tout réglage, maintenance ou réparation doit être effectué comme décrit dans ce manuel, par une personne qualifiée consciente des risques encourus.
2. Il est essentiel que les personnes utilisant et intervenant sur cet appareil respectent les règles de sécurité de travail, en plus des instructions détaillées précisées dans ce manuel.
3. En-dehors des éléments décrits dans les procédures de maintenance ci-inclues, cet appareil ne contient aucun élément réparable par l'utilisateur. L'enlèvement des capots et les tentatives de réglage ou de réparation par des personnes non qualifiées invalide toute garantie et entraîne un risque de frais de réparation supplémentaires.
4. Toujours se référer aux fiches techniques de santé et de sécurité accompagnant tout produit chimique utilisé. Respecter les procédures de laboratoire généralement acceptées pour la manipulation en toute sécurité des produits chimiques.
5. Si l'utilisateur suspecte qu'un problème quelconque puisse mettre en cause la sécurité, l'appareil doit être rendu inopérant en empêchant son utilisation. Communiquer la défaillance constatée au service de maintenance compétent.

Bitte lesen Sie diese Hinweise vor Installation oder Gebrauch dieser Ausrüstung sorgfältig durch.

1. Das in diesem Handbuch beschriebene Gerät darf nur von geschultem Personal bedient werden. Alle Anpassungen, Wartungsarbeiten und Reparaturen müssen entsprechend der Vorgaben in diesem Handbuch und von einer kompetenten Person, die mit den damit verbundenen Gefahren vertraut ist, durchgeführt werden.
2. Es ist wichtig, dass sowohl das Bedienungs- als auch das Service-Personal zusätzlich zu den detaillierten Anweisungen in diesem Handbuch ein sicheres Arbeitssystem einsetzen.
3. Mit Ausnahme der Teile, deren Wartungsverfahren in diesem Handbuch beschrieben sind, enthält dieses Gerät keine weiteren Teile, die vom Benutzer gewartet werden können. Das Entfernen von Abdeckungen und Versuche von hierfür unqualifiziertem Personal, Anpassungen oder Wartungsarbeiten durchzuführen, haben zur Folge, dass die Garantie verfällt und können zusätzliche Reparaturkosten auslösen.
4. Es ist jederzeit auf die sicherheitsrelevanten Daten sämtlicher verwendeter Chemikalien Bezug zu nehmen. Allgemein anerkannte Labormethoden zum sicheren Umgang mit Chemikalien sollten eingesetzt werden.
5. Besteht der Verdacht, dass die Sicherheitsvorrichtungen in irgendeiner Weise beschädigt wurden, muss das Gerät außer Betrieb genommen und gegen weiteren Gebrauch gesichert werden. Die Störung sollte der zuständigen Serviceeinrichtung unverzüglich gemeldet werden.

Leggere attentamente queste istruzioni prima di installare o utilizzare il dispositivo.

1. L'unità descritta nel presente manuale è stata realizzata per essere utilizzata solo da personale che ha ricevuto l'apposita formazione. Qualsiasi operazione di regolazione, manutenzione e riparazione deve essere effettuata sulla base di quanto indicato nel presente manuale da personale qualificato consapevole dei rischi connessi.
2. È fondamentale che il personale operativo e il personale addetto alla manutenzione utilizzino un sistema di lavoro sicuro, oltre a seguire le istruzioni specificate nel presente manuale.
3. Oltre a quelli indicati nelle procedure di manutenzione, all'interno di questo dispositivo non sono presenti altri elementi sui quali è possibile effettuare interventi. La rimozione delle protezioni e qualsiasi tentativo di regolazione o di manutenzione posto in essere da personale non qualificato invaliderà la garanzia. In questi casi, sarà necessario pagare un importo per le riparazioni effectuated.

4. È sempre necessario fare riferimento ai dati sulla salute e sulla sicurezza forniti con le sostanze chimiche utilizzate. Adottare le procedure di laboratorio generalmente accettate per la gestione delle sostanze chimiche.
5. Nel caso in cui si sospetti che la salute possa essere pregiudicata in qualsiasi modo, disattivare l'unità per renderla inutilizzabile. Qualsiasi condizione di errore deve essere immediatamente segnalata al responsabile per la manutenzione.

Lea esta información atentamente antes de instalar o utilizar este equipo.

1. La unidad descrita en este manual está diseñada para que solamente la utilice personal con formación. Cualquier operación de ajuste, mantenimiento y reparación debe llevarse a cabo del modo indicado en este manual y debe realizarla una persona cualificada que sea consciente de los peligros que implica.
2. Es fundamental que tanto los operarios como el personal de servicio utilicen un sistema de trabajo seguro, así como las instrucciones detalladas que se especifican en este manual.
3. Cualquier elemento que no se encuentre entre los definidos en los procedimientos de mantenimiento aquí descritos no podrá utilizarse en este instrumento. La extracción de las tapas y los intentos de ajuste o reparación por parte de personal no cualificado invalidarán la garantía y pueden incurrir en cargos adicionales por reparación.
4. Siempre deberían consultarse los datos sobre Salud y Seguridad que se suministran con cualquier producto químico que se utilice. Es necesario llevar a cabo los procedimientos de laboratorio de aceptación generalizada para la manipulación segura de productos químicos.
5. Si existe la sospecha de que las medidas protectoras de seguridad han quedado dañadas en cualquier modo, la unidad debe inutilizarse y protegerse contra toda operación que se intente llevar a cabo. El estado de fallo debe comunicarse inmediatamente a la autoridad de servicio de mantenimiento y reparación pertinente.

Contents

SECTION 1 – Introduction	8
1.1 INSTRUMENT DESCRIPTION.....	8
1.2 INSTRUMENT SPECIFICATION.....	8
SECTION 2 – Installation	9
2.1 UNPACKING	9
2.2 INSTALLATION	9
2.3 DISPLAY	10
2.4 CONTROLS.....	11
2.5 REAR PANEL.....	13
2.6 FRONT VIEW.....	13
SECTION 3 – THEORY AND PRACTICE OF SPECTROSCOPY MEASUREMENTS	14
3.1 THEORY OF SPECTROSCOPY MEASUREMENT	14
3.2 NUCLEIC ACID DETERMINATION.....	15
3.3 SPECTROSCOPY MEASUREMENT.....	15
3.4 GOOD PRACTICE GUIDELINES	16
SECTION 4 – INSTRUMENT SETUP	18
4.1 INSTRUMENT NAVIGATION.....	18
4.2 MAIN MENU SCREEN	18
4.2.1 Slit Width Setting	18
4.3 SYSTEM UTILITY MENU	19
4.3.1 Wavelength Reset	19
4.3.2 Printer Setup.....	19
4.3.3 Lamp Setup	20
4.3.3.1 Change the Lamp Switch Point	20
4.3.4 Clock Setup	20
4.3.4.1 Set Time	20
4.3.4.2 Set Date.....	21
4.3.4.3 Display Time / Date	21
4.3.5 Refresh Dark Current	21
4.3.6 Connect to PC	21
4.3.7 Beeper On/Off	21
4.3.8 Language Selection.....	21
4.3.9 Refresh System Baseline	21
4.3.10 Delete Entire Saved Files	22
4.3.11 Restore Default Settings.....	22
SECTION 5 – PHOTOMETRICS	23
5.1 PHOTOMETRICS MENU SCREEN	23
5.2 METHOD SET UP	23
5.2.1 Selecting a Wavelength	23
5.2.2 Selecting the Measurement Mode	23
5.2.3 Selecting the Unit of Measurement.....	24
5.2.4 Entering a Concentration Factor	24
5.3 CALIBRATION.....	24
5.3.1 Zero Calibration	24
5.3.2 Calibrating to a Standard	25
5.4 SAMPLE MEASUREMENT	25
5.4.1 Photometric Measurements.....	25

5.4.2	Measuring a Sample after Entering a Concentration Factor	25
5.4.3	Measuring a Sample after Calibrating to a Standard	26
SECTION 6 – QUANTITATION		27
6.1	QUANTITATION MODE SCREEN	27
6.2	WAVELENGTH SELECTION	27
6.3	METHOD SETUP	27
6.3.1	Selecting the Unit of Measurement	28
6.3.2	Quantitation Table Settings	28
6.3.2.1	Select Curve Fit	28
6.3.2.2	Manually Enter Curve Constants	29
6.3.2.3	Edit Calibration Table	29
6.3.2.4	Display Calibration Curve	29
6.4	CREATING A NEW STANDARD CURVE	30
6.5	STORING A STANDARD CURVE	31
6.6	RECALLING A STORED STANDARD CURVE	31
6.7	SAMPLE MEASUREMENTS	31
6.7.1	Quantitation Measurements	32
6.8	STORING RESULTS	32
6.9	RECALLING STORED RESULTS	32
SECTION 7 – SPECTRUM		33
7.1	SPECTRUM MODE SCREEN	33
7.2	METHOD SETUP	33
7.3	SELECTING THE MEASUREMENT MODE	34
7.4	SAMPLE MEASUREMENTS	34
7.5	ADJUSTING THE DISPLAYED SCAN RANGE	34
7.6	SPECTRUM SEARCH	35
7.7	SPECTRUM SMOOTHING	35
7.8	STORING RESULTS	35
7.9	RECALLING STORED RESULTS	36
SECTION 8 – KINETICS		37
8.1	KINETICS MODE SCREEN	37
8.2	WAVELENGTH SELECTION	37
8.3	METHOD SETUP	37
8.3.1	Selecting the Measurement Mode	38
8.4	SAMPLE MEASUREMENTS	38
8.5	ADJUSTING THE DISPLAYED SCAN RANGE	38
8.6	CALCULATING I/U CONCENTRATION	39
8.7	SPECTRUM SMOOTHING	39
8.8	STORING RESULTS	40
8.9	RECALLING STORED RESULTS	40
SECTION 9 – DNA/PROTEIN		41
9.1	DNA MENU OPTIONS	41
9.2	ADJUSTING THE MEASUREMENT MODE	41
9.3	WAVELENGTH SELECTION	42
9.4	ADJUSTING THE CONCENTRATION CALCULATION FACTORS	42
9.5	SELECTING THE UNIT OF MEASUREMENT	42
9.6	RESET MODE SETTINGS	43
9.7	DNA/PROTEIN MEASUREMENTS	43
9.8	STORING METHODS/RESULTS	43
9.9	RECALLING STORED RESULTS	44
SECTION 10 – MULTI-WAVELENGTH		45

10.1	MULTI-WAVELENGTH MODE OPTIONS	45
10.2	WAVELENGTH SELECTION	45
10.3	SAMPLE MEASUREMENT	46
10.4	STORING METHODS/RESULTS	46
10.5	RECALLING STORED RESULTS	46
SECTION 11 – SAVING/RECALLING RESULTS USING A USB MEMORY STICK		47
SECTION 12 – ACCESSORIES AND SPARE PARTS		48
12.1	OPTIONAL ACCESSORIES	48
12.2	INSTALLING THE PASSIVE AND ACTIVE ACCESSORIES	48
12.2.1	Passive Accessories	48
12.2.2	Active Accessories	49
12.2.2.1	8 Position Automatic Cell Changer	49
12.3	USING THE 8 POSITON AUTOMATIC CELL CHANGER	50
12.4	SPARES	51
SECTION 13 – MAINTENANCE AND SETVICE		51
13.1	ROUTINE MAINTENANCE	51
13.2	LAMP REPLACEMENT	51
13.2.1	Tungsten Lamp Replacement	51
13.2.2	Deuterium Lamp Replacement	52
13.3	SERVICE	53
SECTION 14 – TROUBLESHOOTING		54
14.1	TROUBLESHOOTING GUIDE	54
14.2	TECHNICAL SUPPORT	54
SECTION 15 – DECLARATION OF CONFORMITY		55

SECTION 1 – Introduction

1.1 INSTRUMENT DESCRIPTION

The SP-800-UV is a variable bandwidth, double beam UV/visible spectrophotometer with an integrated user interface for local control. This instrument has highly stable optics and two detectors that measure the sample and reference solutions simultaneously to optimise the accuracy of the measurement. The SP-800-UV has measurement modes for photometrics, concentration, multi-wavelength, spectrum scanning, quantitation, kinetics and DNA and Protein analysis. The instrument is supplied with Cole-Parmer Prism PC software to allow full PC control of the spectrophotometer.

1.2 INSTRUMENT SPECIFICATION

SP-800-UV	
Wavelength	
Range	190 to 1100nm
Resolution	0.1nm
Accuracy	± 0.3nm (at 0.5 and 1nm bandwidth) ± 0.5nm (at 2, 4 and 5nm bandwidth)
Repeatability	± 0.2nm
Spectral bandwidth	Variable 0.5 / 1 / 2 / 4 and 5nm
Photometrics	
Transmittance	0 to 200%
Absorbance	-0.3 to 3.0A
Accuracy	±0.3%T (0 – 100%T), ±0.002A (0 – 0.5A)
Reproducibility	±0.001 Abs (0 to 0.5 Abs) ±0.002 Abs (0.5 to 1.0 Abs)
Resolution	0.1%T, 0.001A
Stray light	<0.05% at 360nm and 220nm
Noise	0.0005A
Stability	±0.001A at 500nm after 15min warm up
Quantitation	
Range	0 to 99999
Data points	Up to 3 wavelengths
Calibration	Blank with up to 10 standards
Units	IU, mM/L, M/L, µg/mL, mg/mL, mg/L, mEq, ppb, ppm, % and other
Curve fit algorithms	Linear, Linear through zero, Quadratic and Cubic
Multi-wavelength	
Range	0 to 99999
Data points	Up to 10 wavelengths
Kinetics	
Measurement Time	Up to 12 hours
Scan Interval	0.1, 0.2, 0.5, 1, 2, 5, 10 or 30 seconds
Calibration	Blank with a single standard or factor
Display	Graphical and concentration
Analysis	Slope and line of best fit between any two points
Spectrum	
Range	Any range between 190 to 1100nm
Scan speed	100 to 2000nm/min
Scan interval	Selectable 0.1, 0.2, 0.5, 1, 2 or 5nm
DNA	
Measurement modes	DNA/RNA Ratio, concentration, A320 correction

Protein	
Measurement modes	Direct UV
Other	
Beam height	15mm
Light source	Tungsten and Deuterium lamps
Outputs	USB, Parallel (Printer)
Power	110/220V AC 50/60Hz
Size (w x d x h)	600 x 450 x 260mm
Weight	22kg

SECTION 2 – Installation

2.1 UNPACKING

Remove the SP-800-UV from the packaging and ensure the following items are included:

1. Model SP-800-UV spectrophotometer fitted with 10 x 10mm cuvette holder
2. Power supply cables – UK lead
– EU lead
– US lead
3. Instruction manual
4. 10mm Glass Cuvettes x 4
5. 10mm Quartz Cuvettes x 2
6. Dust Cover
7. PC software CD and USB security dongle

2.2 INSTALLATION

The SP-800-UV is supplied ready to use.

The working temperature and humidity range of the SP-800-UV spectrophotometer is 15 – 35°C, 15 – 70% relative humidity. The storage temperature and humidity range of the SP-800-UV spectrophotometer is -10 – 50°C, 15 – 70% relative humidity.

The unit should be placed on a clean flat surface which is free from drafts and vibrations. The units are designed for operation on 110V±11V / 60Hz±1Hz and 220V±22V / 50Hz±1Hz AC.

Connect the power supply unit to the power inlet socket on the rear panel of the instrument and connect to the mains socket. Turn the power on at the mains and switch the instrument on using the power switch on the rear of the instrument.

The instrument will initially perform several power-on tests before displaying the warm up screen:



Fig 2.2 – Instrument power-on tests complete

The power-on tests comprise

1. Lamp test
2. Detector test
3. A to D converter test
4. Grating position check
5. Dark current check

2.3 DISPLAY

The instrument has an inclusive display which enables text and graphs to be displayed clearly. Following successful completion of the power-on tests and the instrument warm up time, the main menu screen will be displayed:

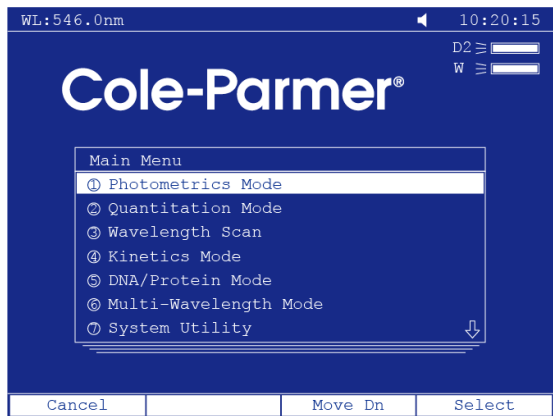


Fig. 2.3 – Display

Main menu options

1. Photometrics measurement mode
2. Quantitation measurement mode
3. Spectrum measurement mode
4. Kinetics measurement mode
5. DNA/Protein measurement mode
6. Multi-wavelength measurement mode
7. Instrument settings menu
8. Slit width

2.4 CONTROLS

The keypad used for this model enables an easy and effective way of navigating the different measurement modes, entering numbers, saving and analysing results. The keypad is displayed below.


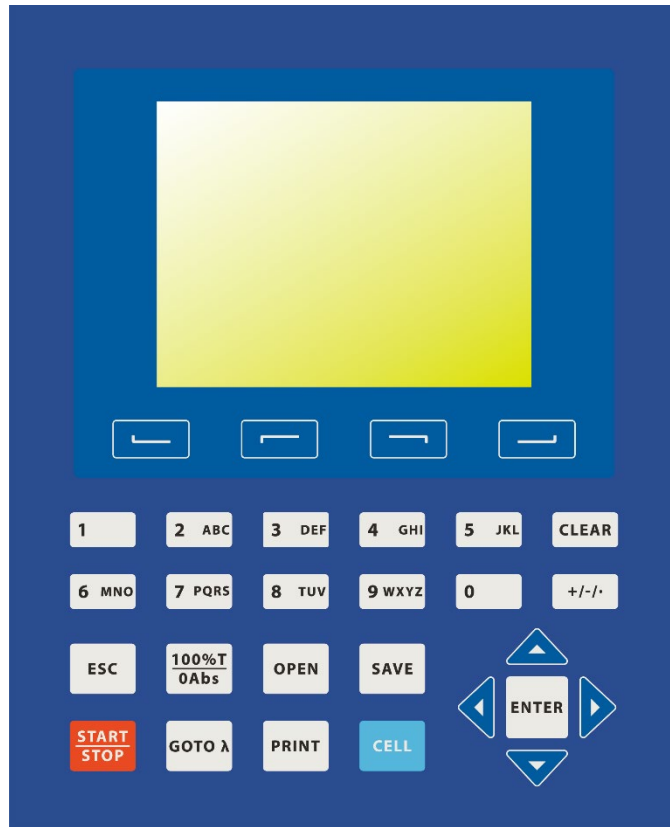


Fig. 2.4 – Keypad



Function Keys: Allows on-screen options to be selected



Numeric Keys: Enter numbers and letters. Select corresponding menu options.




CLEAR Key: Delete the entered value or stored data



BACK Key: Delete a single character



ESC Key: Return to previous menu screen



100%T/0Abs Key: Zero / Blank instrument



OPEN Key: Open results stored in internal memory



SAVE Key: Save results to internal memory



START/STOP Key: Start/Stop measurement



GOTO λ Key: Set the instrument wavelength using the numeric keys. Press the Enter key to confirm.



PRINT Key: Print result




ENTER Key: Confirm operation



CELL Key: Select/Deselect Auto-cell Holder position (If fitted). Use the numeric keys (1-8) to move to cell holder to the corresponding cell position



RIGHT, LEFT Keys: Search peak/valley and set X axis scale



UP, DOWN Keys: Scroll menu/data and set Y axis scale

2.5 REAR PANEL

The image below shows the rear panel of the instrument:



Fig. 2.5 – Rear Panel

- | | |
|----------------------------|-----------------------------------------------------|
| 1. Fan Cover | Allows access to lamp when replacement is necessary |
| 2. Power switch | On/off switch for the unit |
| 3. Power in socket | Connection socket for power supply unit |
| 4. LCD contrast adjustment | Connection to a PC or external serial printer |
| 5. Parallel port | Allows the accessory printer to be connected |
| 6. USB port | Allows the instrument to be connected to a PC |

2.6 FRONT VIEW

The image below shows the front view of the instrument:



Fig. 2.6 – Front Panel

1. LCD display
2. Keypad
3. Sample chamber lid
4. Sample chamber

SECTION 3 – THEORY AND PRACTICE OF SPECTROSCOPY MEASUREMENTS

3.1 THEORY OF SPECTROSCOPY MEASUREMENT

UV-visible spectroscopy is the measurement of the absorbance of light at a specific wavelength in a sample. This is used to identify the presence and concentration of molecular entities within the sample. The Beer-Lambert law is used to relate the absorption of light to the properties of the sample through which the light is travelling through. The Beer-Lambert law states that:

$$A = \epsilon l c$$

A is the absorbance


ϵ is the molar absorption coefficient ($\text{l mol}^{-1}\text{cm}^{-1}$)

c is the concentration (mol l^{-1})

l is the path length (cm)

This law shows that absorbance is linear to concentration but this is only true for low concentrations. For absorbance levels above 3 the concentration starts to move away from the linear relationship.

Transmittance is the proportion of the light which passes through the sample:

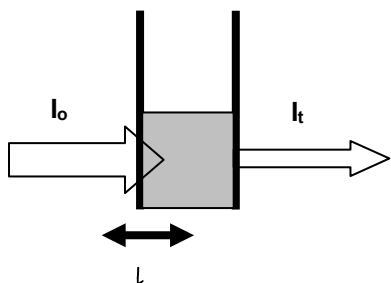

Where:

I_o is the incident light

I_t is the transmitted light

l is the path length

Therefore:

$$T = \frac{I_t}{I_o}$$

Absorbance is inversely related to transmittance:

$$A = \log \frac{1}{T}$$

3.2 NUCLEIC ACID DETERMINATION

DNA, RNA and oligonucleotides can be measured directly in aqueous solutions in a diluted or undiluted form. Aqueous buffers with low ion concentrations (e.g. TE buffer) are ideal for this method. The concentration is commonly determined by measuring at 260nm against a blank and then evaluating against a factor.

The SP-800-UV has pre-defined methods installed which assume that absorption of 1 OD (A) is equivalent to, approximately: 50µg/ml dsDNA, 37µg/ml ssDNA, 40µg/ml RNA and 30µg/ml for oligonucleotides.

DNA interference by contaminants can be assessed by the calculation of an absorption ratio. The ratios A260/A280 and A260/A230 are used to estimate the purity of nucleic acids, since proteins absorb at 280nm and substances such as peptides, phenols, aromatic compounds or carbohydrates absorb at 230nm. Pure DNA should have an A260/A280 ratio of approximately 1.8 and pure RNA 2.0. In pure nucleic acid samples the A260/A230 ratio should be approximately 2.2.

Nucleic acid concentration can also be estimated with the following calculations:

$$\text{Conc } (\mu\text{g/ml}) = (\text{Abs}@260\text{nm} \times 62.9) - (\text{Abs}@280\text{nm} \times 36.0)$$

$$\text{Conc } (\mu\text{g/ml}) = (\text{Abs}@260\text{nm} \times 49.1) - (\text{Abs}@230\text{nm} \times 3.48)$$

Referring to a blank value where no absorption should occur is commonly required. On the SP-800-UV the default reference wavelength is 320nm and the user can include the measured absorbance value in all nucleic acid calculations. The default wavelength can be modified from 320nm if required.

3.3 SPECTROSCOPY MEASUREMENT

There are four main components of a spectrophotometer. These are a light source to emit a high and constant amount of energy over the full wavelength range; a method for separating the light into discrete wavelengths; a sample holder and a light detector.

The optical layout of the SP-800-UV spectrophotometer is shown overleaf:

The light from the tungsten and deuterium lamps is focused onto the grating which separates the light into discrete wavelengths. The diffracted spectrum of light then passes through a further slit and lens arrangement before passing through a beam splitter which directs half of the light towards the sample holder and half towards the reference sample holder. The light which is not absorbed by the two solutions is transmitted through a collecting lens and onto the signal detector. The signal from each photo-diode detector is used to calculate the % transmittance. The result is displayed either as % transmittance or absorbance on the instrument display.

3.4 GOOD PRACTICE GUIDELINES

1. For optimum performance all spectrophotometers should be sited in a clean, dry, dust free atmosphere. When in use ambient temperature and light levels should remain as constant as possible.
2. If required adherence to Standard Operating Procedures (SOP) and Good Laboratory Practice (GLP) should be monitored with regular calibration checks and a suitable Quality Control (QC) programme.
3. The sample chamber lid must be fully closed during measurement and before any readings are recorded or printed.
4. The correct selection of sample containers is imperative for accurate and reproducible results:
 - a) Check that the material of the sample container is compatible with the wavelengths to be used for measurement. In general glass can only be used down to 360nm or 320nm depending on quality. Standard plastic cuvettes can be used down to 320nm. Special UV versions can be used down to 260nm. Below this level quartz cuvettes must be used.
 - b) Plastic disposable cuvettes should only be used ONCE.
 - c) Glass cuvettes should be thoroughly cleaned after use. Discard when scratches become evident on optical surfaces.
 - d) Care should be taken when selecting semi-micro or micro cuvettes. The cuvette window on the inner chamber (the area filled with sample) must be wider than the aperture in the sample holder or light will reach the detector without passing through the sample. In this case, semi-micro or micro cuvettes with self-screening black surrounds must be used or, alternative holders for these cuvettes should be used.
 - e) Glass test tubes and other sample tubes should be used with care. Where possible, matched tubes should be used and any index mark set to the correct position before measurements are made.
 - f) Ensure any sample containers used are compatible with the constituents of both the samples and standards they are to hold. Plastic cuvettes are not compatible with organic solvents.
 - g) All sample containers must be handled with care; by the top, bottom and non-optical surfaces only. Any finger marks evident must be removed by a suitable cleaning process.


- h) Flow-through cuvettes must be selected with care and consideration for the sample type, sample volume, pumping system, rinse, sample and waste handling to be used.
5. Samples and standards should not be stored in open cuvettes or sample containers as evaporation will change the value and lead to staining of the walls which may be irreversible. If stored in stoppered and sealed cuvettes, they should be filled with little or no air space and the values regularly checked against a reference standard or quality control material.
 6. Samples should be allowed to equilibrate to ambient temperature before measurement (unless a suitable temperature controlled sample holder is in use). Temperature change during measurement may cause air bubbles to form on the walls of the sample holder. This is a common cause of drift during measurement.
 7. In the preparation of samples and standards high grade borosilicate glass and AR grade chemicals and reagents must be used. Good quality deionised water or other suitable solvents must be used for dissolving or diluting samples, chemicals and reagents.
 8. All measurements require calibration to a blank, for maximum accuracy this should be prepared with care using the same deionised water or solvent used for dissolving or diluting the sample. Where reagents are added to the sample to produce a colour proportional to its concentration a 'sample based' blank should be used. In this case the blank should consist of all reagents or chemicals to be used, **except** the sample which will produce the colour to be measured.
 9. Deviations from the Beer-Lambert Law may occur at high and low concentrations giving non-linear response during sample concentration measurements. For all new methods a linear range should be defined by the preparation of a calibration curve. The quantitation mode may be used to construct such a curve against which sample results are automatically measured.
 10. Cuvettes and sample holders must be filled to a minimum level which covers the light path. All Cole-Parmer spectrophotometers have a beam height of 15mm.
 11. The instrument must be calibrated to zero absorbance/100% transmittance prior to taking readings. In the spectrum measurement mode a baseline scan must be performed before performing a sample scan.

SECTION 4 – INSTRUMENT SETUP

4.1 INSTRUMENT NAVIGATION

To navigate around the spectrophotometer screen press the arrow keys on the main keypad and use the Enter key to select the highlighted option. Alternatively, some options and actions require the user to press the function and numeric keys on the instrument keypad. The Esc key can be used to return to the previous menu without saving any changes.

4.2 MAIN MENU SCREEN

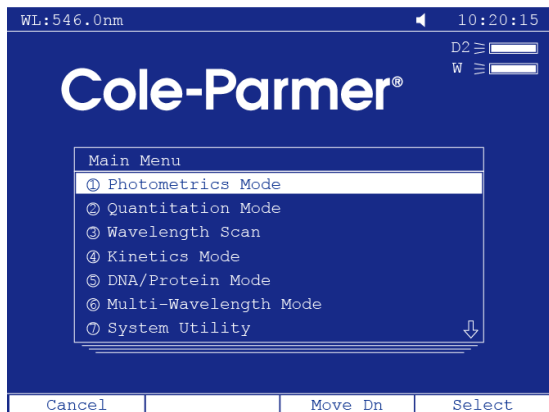

Main Menu Screen


The main menu screen provides access to all measurement modes, the system utility menu and the variable slit width setting. The available measurement modes are photometrics, quantitation, spectrum scan, kinetics, DNA/Protein and multi-wavelength.

The system utility menu option allows the user to perform a variety of setup and service functions. See section 4.3 for further details on these options.

4.2.1 Slit Width Setting

The slit width option allows the user to select the instrument's bandwidth parameter from the available options 0.5, 1.0, 2.0, 4.0 and 5.0 nm. Use the arrow keys to cycle through the options and press the Enter key to confirm. The instrument will perform a dark current calibration before returning to the main menu.

4.3 SYSTEM UTILITY MENU

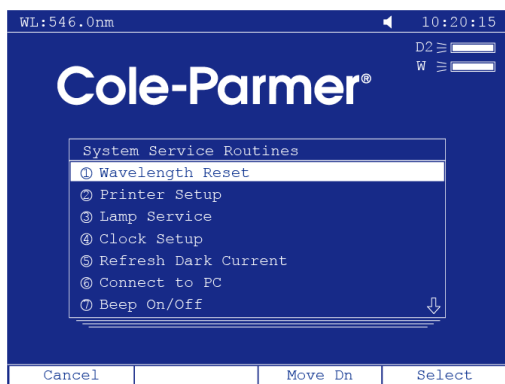

System Utility Menu


The system utility menu option allows the user to perform a variety of setup and service functions.

1. Wavelength calibration
2. Edit printer settings
3. Edit lamp settings
4. Edit time and date settings
5. Measure the instrument's dark current
6. Connect to a PC
7. Edit keypad sound options
8. Set the displayed language
9. Perform a system baseline measurement
10. Perform an instrument reset

4.3.1 Wavelength Reset

Highlight the wavelength reset option and press the Enter key to confirm. This will recalibrate the wavelength setting of the instrument. Once complete the instrument will return to the System Utility menu.

4.3.2 Printer Setup

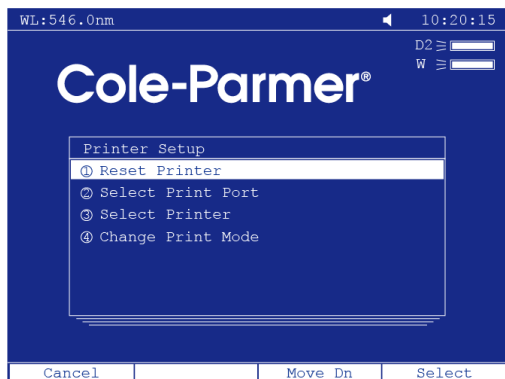


In the printer setup menu the user can perform the following tasks.

1. Reset printer
2. Select print output port (Comm or Lpt)
3. Select printer type
4. Change print mode (Report or Screen Shot)

Highlight the required option using the up and down arrow keys and press the Enter key to confirm.

4.3.3 Lamp Setup

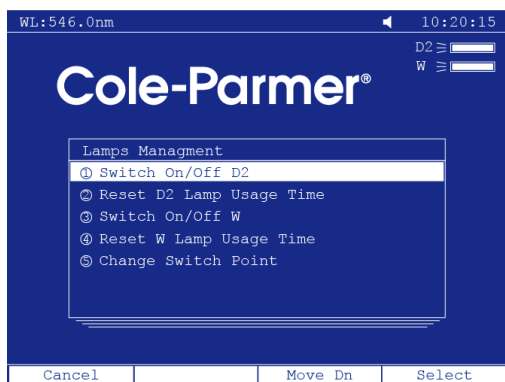

In the lamp setup menu the user can perform the following tasks.


1. Switch on/off the deuterium lamp
2. Reset the deuterium lamp usage timer
3. Switch on/off the tungsten lamp
4. Reset the tungsten lamp usage timer
5. Change the lamp switch point.

Highlight the required option using the up and down arrow keys. Press the Enter key to confirm.

4.3.3.1 Change the Lamp Switch Point

Highlight the Change the lamp switch point option and press the Enter key to confirm. This will allow the user to enter the wavelength where the instrument will switch between the deuterium and tungsten lamps. Enter a wavelength between 300 and 360 nm and press the Enter key to confirm. Once complete the instrument will return to the Lamp Setup menu.

4.3.4 Clock Setup

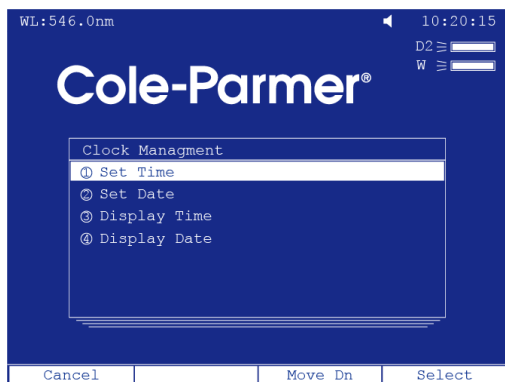

In the clock setup menu the user can perform the following tasks.

1. Set time
2. Set date
3. Display time
4. Display date

Highlight the required option using the up and down arrow keys. Press the Enter key to confirm.

4.3.4.1 Set Time

Highlight the set time option and press the Enter key to confirm. This will allow the user to enter the current time using the numerical keypad and the decimal point keys. Press the Enter key to confirm. Once complete the instrument will return to the Lamp Setup menu.

4.3.4.2 Set Date

Highlight the set date option and press the Enter key to confirm. This will allow the user to enter the current date in the format DD.MM.YY using the numerical keypad and the decimal point keys. Press the Enter key to confirm. Once complete the instrument will return to the Clock Setup menu.

4.3.4.3 Display Time / Date

Highlight the display time or display date option and press the Enter key to confirm. This will set the top right hand corner to show the selected option.

4.3.5 Refresh Dark Current

Highlight the refresh dark current option and press the Enter key to confirm. This will re-measure and store the detectors' dark current values.

4.3.6 Connect to PC

Connect the interface cable to the USB type B port on the rear of the instrument and connect to a USB port on the PC. The connecting COM port should be configured with the following settings:

38400 baud	8 data bits
No parity	1 stop bit

Highlight the Connect to PC option and press the Enter key to confirm.

4.3.7 Beeper On/Off

Highlight the beeper on/off option and press the Enter key to confirm. An audible sound will be heard each time an instrument button is pressed when this option is enabled.

4.3.8 Language Selection

Not currently available.

4.3.9 Refresh System Baseline

Ensure the sample chamber is empty, highlight the refresh system baseline option and press the Enter key to confirm. This will re-measure and store the detectors' signals over the full wavelength range of the instrument.

4.3.10 Delete Entire Saved Files

Highlight the delete entire saved files option and press the Enter key to confirm. A warning will be shown on screen and the user will need to confirm this command again by selecting the Yes option with the up and down arrow keys. This action will delete all saved results and methods from the instrument.

4.3.11 Restore Default Settings

Highlight the restore default settings option and press the Enter key to confirm. This will reset all instrument parameters back to their original factory settings.

SECTION 5 – PHOTOMETRICS

The photometrics measurement mode enables simple measurements of absorbance, % transmittance and concentration to be performed. In this measurement mode it is possible to calibrate against a standard of a known concentration or use a known factor. The sample is measured at one wavelength at one point in time. There are no post measurement calculations available in this measurement mode.

5.1 PHOTOMETRICS MENU SCREEN



The photometrics measurement mode screen enables measurement parameters to be changed. The four options at the bottom of the screen allow the user to select the unit of measurement, the measurement mode, the concentration factor and the calibration standard's concentration. These options are selected with the corresponding function buttons.

5.2 METHOD SET UP

The photometrics measurement mode is very simple and the only parameters which can be adjusted are the wavelength, the units of the measurement the measurement mode and the concentration setup parameters.

5.2.1 Selecting a Wavelength

The wavelength can be adjusted by pressing the GOTO λ key on the instrument keypad. The required wavelength can then be entered using the numerical keypad. Press the Enter key to confirm.


5.2.2 Selecting the Measurement Mode

The measurement mode can be selected by pressing the function key below the Mode option. The required measurement mode can then be selected from the available options of Abs, %T and Conc/Factor using the up and down arrow keys. Press the Enter key to confirm.

5.2.3 Selecting the Unit of Measurement

The unit of measurement can be selected by pressing the function key below the Unit option. The required unit of measurement can then be selected from the available options of IU, mM/L, M/L, µg/mL, mg/mL, mg/L, mEq, ppb, ppm, % and other. Press the Enter key to confirm.

5.2.4 Entering a Concentration Factor

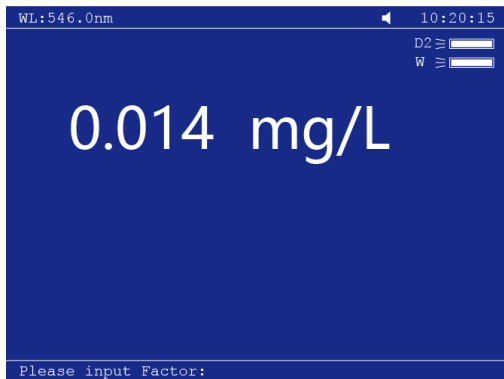

The concentration of a sample can be determined by using an appropriate multiplication factor with the measured photometric reading. A concentration factor can be entered by pressing the function button below the Factor option. The required factor can then be entered using the numerical keypad. Press the Enter key to confirm.


5.3 CALIBRATION

5.3.1 Zero Calibration



A zero calibration can be performed at the same wavelength at which the sample will be measured. With both the reference a sample positions empty and the sample chamber lid closed, press the 100%T/0Abs button to zero the instrument's photometric reading.

5.3.2 Calibrating to a Standard

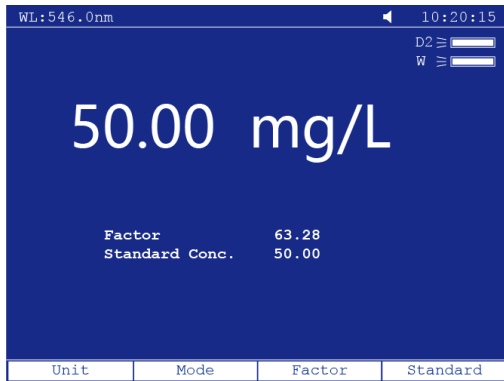

A calibration standard can be used to determine the concentration factor. Insert the cuvette containing the blank solution into the reference position in the sample chamber and insert the cuvette containing the standard solution into the sample position. Close the instrument lid. The concentration of the calibration standard is entered by pressing the function button below the Standard option. The concentration of the calibration standard can then be entered using the numerical

keypad. Press the Enter key to confirm. The concentration factor is then updated on the screen.


5.4 SAMPLE MEASUREMENT

5.4.1 Photometric Measurements



Insert the cuvette containing the blank solution into the reference position in the sample chamber and insert the cuvette containing the sample solution into the sample position. Close the instrument lid and the photometric result will be shown on the screen.


5.4.2 Measuring a Sample after Entering a Concentration Factor

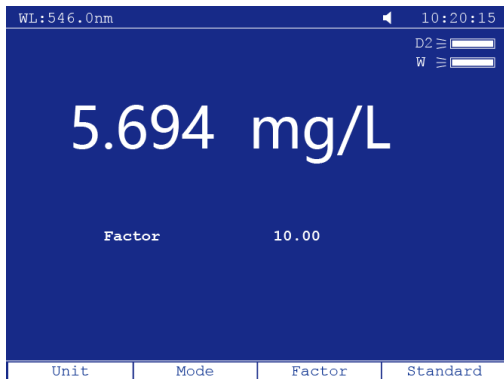

Remove the cuvette containing the blank solution and place a cuvette containing the sample to be measured in the sample chamber. Close the instrument lid and the concentration value will be shown on the screen.

In order to measure a sample based on a known factor the value for the factor must be entered in the settings before commencing measurement of the sample.

5.4.3 Measuring a Sample after Calibrating to a Standard

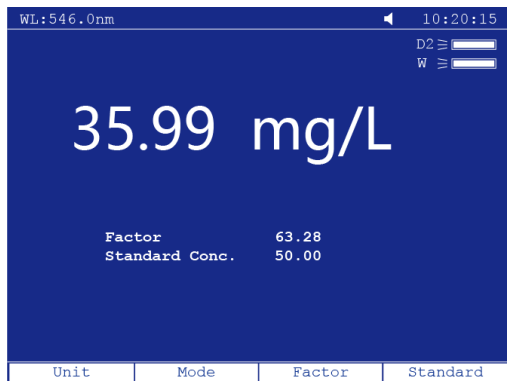


Remove the cuvette containing the standard sample and place a cuvette containing the sample to be measured in the sample chamber. Close the instrument lid and the calculated concentration value will be shown on the screen.

SECTION 6 – QUANTITATION

The quantitation measurement mode enables sample concentrations to be calculated using a standard curve. In this mode a number of standard solutions covering a range of known concentrations are measured. The absorbance or % transmittance of these solutions is plotted to create a standard curve. Once the standard curve has been created a sample of unknown concentration can be measured and the concentration calculated using the standard curve.

6.1 QUANTITATION MODE SCREEN

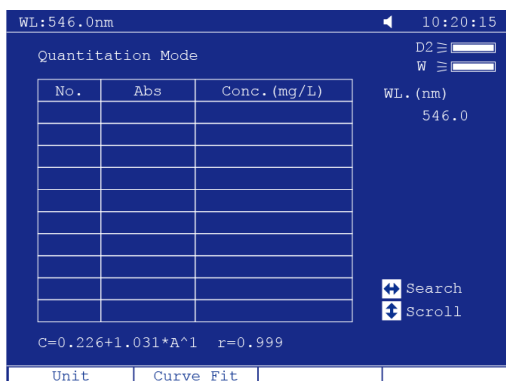

The quantitation measurement mode enables measurement parameters to be changed. The two options at the bottom of the screen allow the user to select the unit of measurement and edit the calibration standard settings. These options are selected with the corresponding function buttons.

6.2 WAVELENGTH SELECTION

The wavelength can be adjusted by pressing the GOTO λ key on the instrument keypad. The user can select from the following options:

1. Single WL

2. Isobestic where $Abs = Abs_{\lambda 1} - Abs_{\lambda 2}$

3. 3 Points where: $Abs = Abs_{\lambda 2} - \left(\frac{m \times Abs_{\lambda 1} + n \times Abs_{\lambda 3}}{m + n} \right)$
 $m = Abs_{\lambda 3} - Abs_{\lambda 2}$ and $n = Abs_{\lambda 2} - Abs_{\lambda 1}$

The required wavelength values can then be entered using the numeric keypad. Press the Enter key to confirm.


6.3 METHOD SETUP

In this measurement mode the method setup parameters are accessed by pressing the function keys below the two options on the quantitation menu screen.

6.3.1 Selecting the Unit of Measurement

The unit of measurement can be selected by pressing the function key below the Unit option. The required unit of measurement can then be selected from the available options of IU, mM/L, M/L, µg/mL, mg/mL, mg/L, mEq, ppb, ppm, % and other. Press the Enter key to confirm.


6.3.2 Quantitation Table Settings

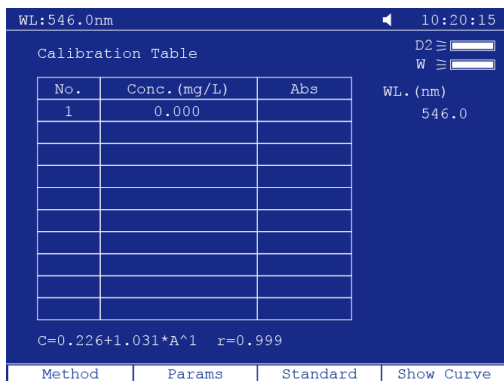

The quantitation table settings are accessed by pressing the function key below the Curve Fit option in the quantitation mode screen. Four new options are available in the quantitation table screen:

4. Method (Change the curve fit algorithm)
5. Params (Enter linear regression constants)
6. Standard (Edit calibration table data)
7. Show Curve (Display calibration curve)

6.3.2.1 Select Curve Fit

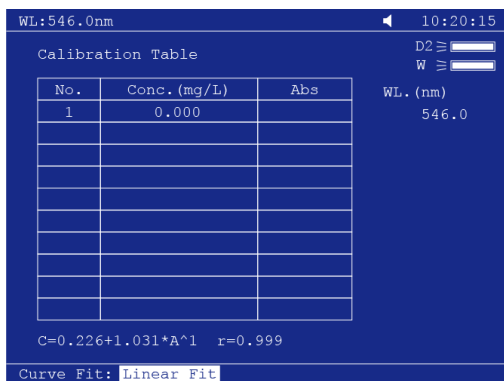


The curve fit algorithm can be selected by pressing the function key below the Method option. Four curve fit options are available:

1. Linear Fit
2. Square Fit (Quadratic)
3. Cubic Fit
4. Linear Fit Through Zero

The required option can be selected using the up and down arrow keys. Press the Enter key to confirm.

6.3.2.2 Manually Enter Curve Constants

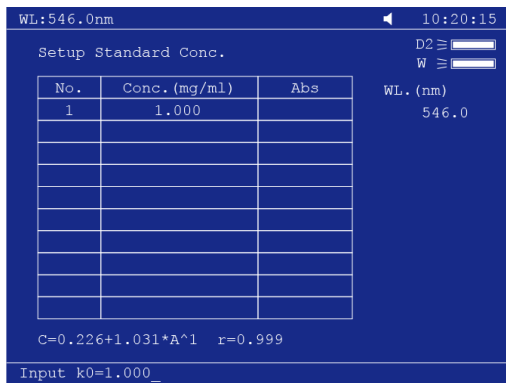


The user can manually enter the calibration curve constants by pressing the function key below the Params option. The user will be prompted to enter the constants that are required for the selected curve fit algorithm.

1. Linear Fit = $K_0 + (K_1 \times \text{Abs})$
2. Square Fit = $K_0 + (K_1 \times \text{Abs}) + (K_2 \times \text{Abs}^2)$
3. Cubic = $K_0 + (K_1 \times \text{Abs}) + (K_2 \times \text{Abs}^2) + (K_3 \times \text{Abs}^3)$
4. Linear Fit Through Zero = $K_1 \times \text{Abs}$

The values can be entered using the numerical keypad. Press the Enter key to confirm.

6.3.2.3 Edit Calibration Table

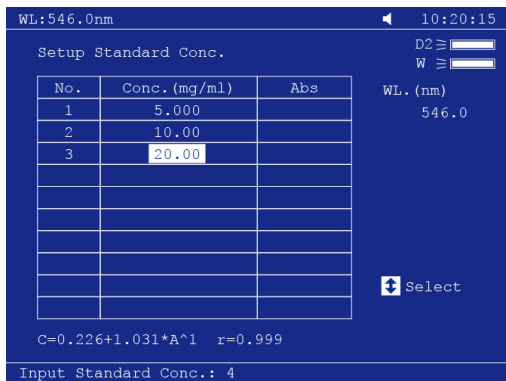

The user can edit the calibration curve data by pressing the function key below the Standard option. The user will be prompted to enter the concentration values for each standard. The values can be entered using the numerical keypad. Press the Enter key to confirm.


To add additional standard values to the table, press the down arrow on the keypad. Once all values have been entered, press the Esc key on the keypad to return to the calibration table settings screen.

6.3.2.4 Display Calibration Curve


Completed calibration curves can be viewed graphically by pressing the function key below the Show curve option.

6.4 CREATING A NEW STANDARD CURVE


The user must firstly edit the calibration table before attempting to create a new standard curve.

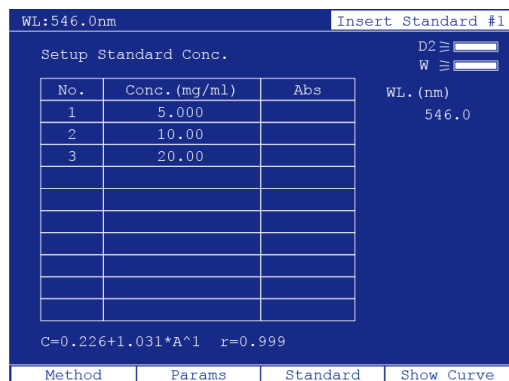

Insert the cuvette containing the blank solution into the reference position in the sample chamber and insert the cuvette containing the first standard solution into the sample position. Close the instrument lid and press the start/stop button. Once the measurement is complete the instrument will ask for the second standard solution to be inserted. Repeat the measurement procedure for each standard solution.

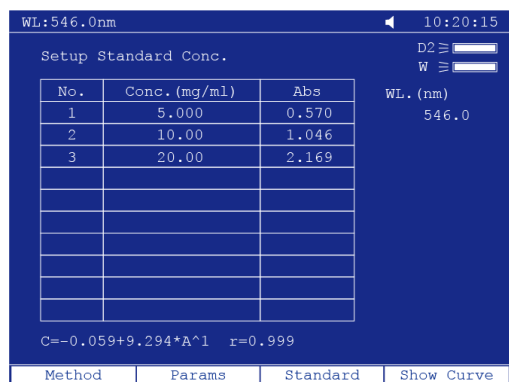


Once all standard solutions have been measured the new standard curve and curve equation will be shown.

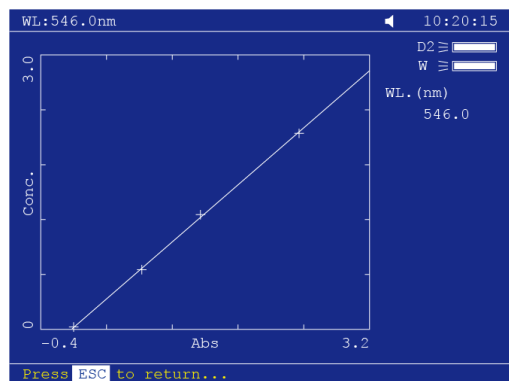

The standard curve can be viewed graphically by pressing the function key below the show curve option on the calibration table screen.


6.5 STORING A STANDARD CURVE

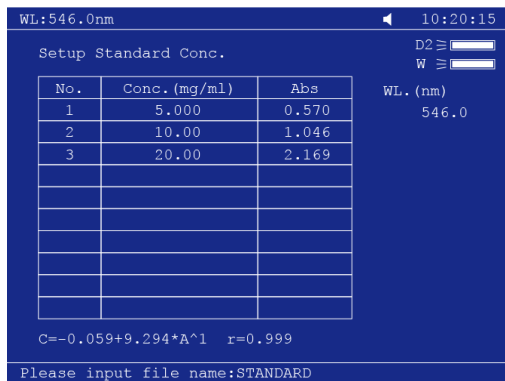

A standard curve can be saved to the instrument's internal memory to allow it to be recalled for future use.

In the calibration table screen press the Save key on the instrument keypad. The instrument will ask the user to enter a filename (max. 8 characters) using the alphanumeric keypad. The user can select the indicated letters, numbers and symbols by repeatedly pressing the key until the required value is displayed, after a short period the next character can be entered in the same manner. Once the filename has been entered, press the Enter key to confirm.

6.6 RECALLING A STORED STANDARD CURVE

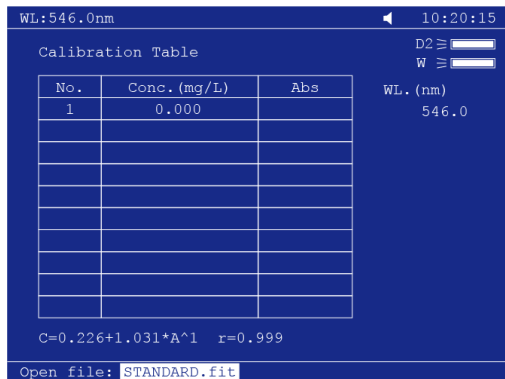


A standard curve can be opened from the instrument's internal memory to allow it to be re-used for sample quantification.

In the calibration table screen press the Open key on the instrument keypad. The user can select from the list of stored files by pressing the up and down arrow keys. Once the required file has been located press the Enter key to confirm.

6.7 SAMPLE MEASUREMENTS


The user should ensure that the appropriate standard curve data has been measured or recalled and that the instrument is displaying the quantitation mode screen before performing a sample measurement.

6.7.1 Quantitation Measurements

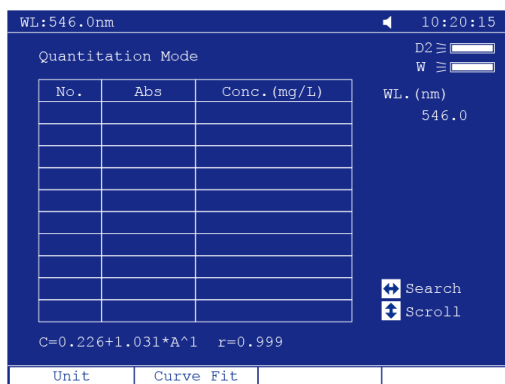

Ensure that a cuvette containing the blank solution is in the reference position in the sample chamber and insert the cuvette containing the sample solution into the sample position. Close the instrument lid and press the Start/Stop key on the keypad. Once the measurement is complete the determined result will be displayed in the quantitation mode screen. Further samples can be measured in a similar manner.


6.8 STORING RESULTS

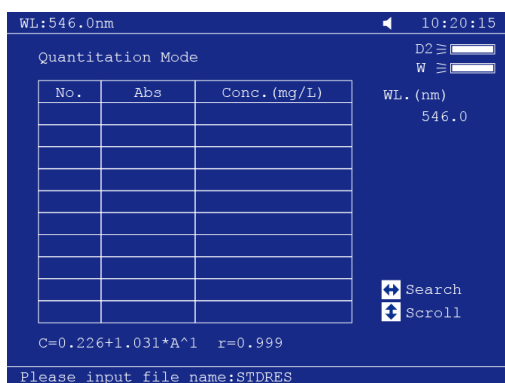

A result file can be saved to the instrument's internal memory.

In the quantitation mode screen press the Save key on the instrument keypad. The instrument will ask the user to enter a filename (max. 8 characters) using the alphanumeric keypad. The user can select the indicated letters, numbers and symbols by repeatedly pressing the key until the required value is displayed, after a short period the next character can be entered in the same manner. Once the filename has been entered, press the Enter key to confirm.

6.9 RECALLING STORED RESULTS

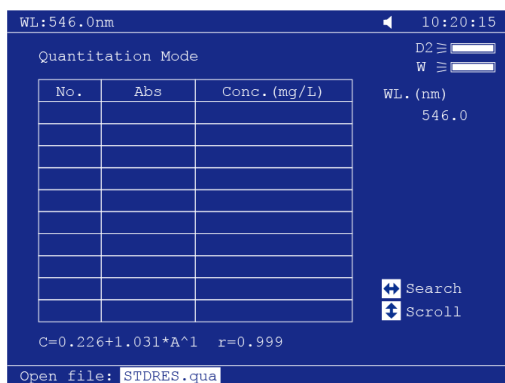


A result file can be opened from the instrument's internal memory.

In the quantitation mode screen press the Open key on the instrument keypad. The user can select from the list of stored files by pressing the up and down arrow keys. Once the required file has been located press the Enter key to confirm.

SECTION 7 – SPECTRUM


The spectrum measurement mode enables measurements of absorbance or % transmittance over a range of wavelengths to be performed. The absorbance or % transmittance at each wavelength is plotted graphically. Post measurement tools such as peaks and spectral points analysis can be performed. This operating mode can be used to partially characterise a sample.

7.1 SPECTRUM MODE SCREEN

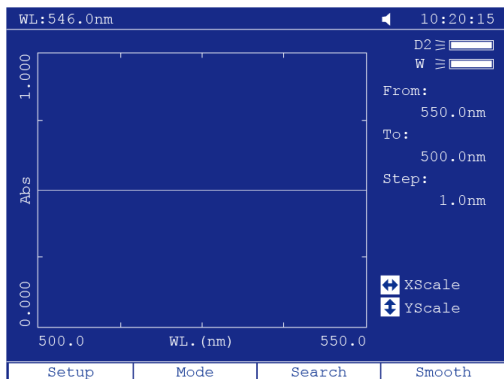

The spectrum measurement mode enables measurement parameters to be changed and post measurement tools to be accessed. The four options at the bottom of the screen allow the user to edit the scan settings, select the measurement mode, perform a post measurement search of the spectrum or apply a smoothing algorithm to the displayed scan. These options are selected with the corresponding function buttons.

7.2 METHOD SETUP

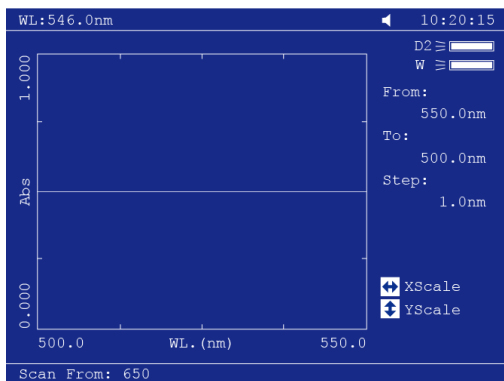

The spectrum scan settings can be edited by pressing the function key below the Setup option. The options that can be changed are:-


1. Scan from (Highest Wavelength)
2. Scan to (Lowest Wavelength)
3. Scan Interval
4. Scan Speed

The numeric keypad should be used to enter the required start and end wavelengths and the up and down arrow keys are used to select from the available scan interval and scan speed options. Press the Enter key to confirm.

7.3 SELECTING THE MEASUREMENT MODE


The measurement mode can be selected by pressing the function key below the Mode option. The required measurement mode can then be selected from the available options of Abs and %T using the up and down arrow keys. Press the Enter key to confirm.

7.4 SAMPLE MEASUREMENTS

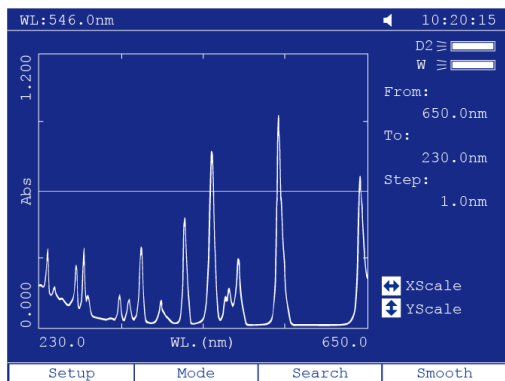


Insert a cuvette containing the blank solution into the reference position in the sample chamber and insert the cuvette containing the sample solution into the sample position. Close the instrument lid and press the Start/Stop key on the keypad. Once the measurement is complete the measured spectrum scan will be displayed on the screen.

7.5 ADJUSTING THE DISPLAYED SCAN RANGE

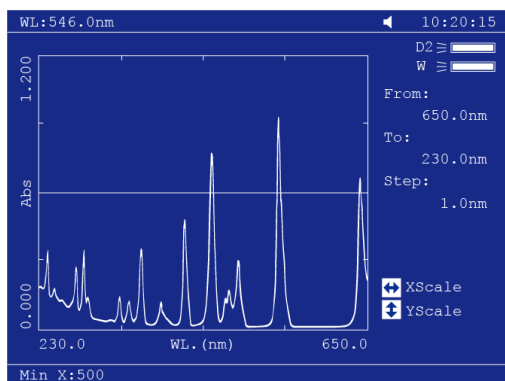


The instrument will display the full range scan after a measurement is complete. To change the displayed wavelength range, press the left or right arrow keys. The minimum and maximum display wavelengths can be entered using the numeric keypad. Press the Enter key to confirm. To change the displayed photometric range, press the up or down arrow keys. The minimum and maximum values can be entered using the numeric keypad. Press the Enter key to confirm.

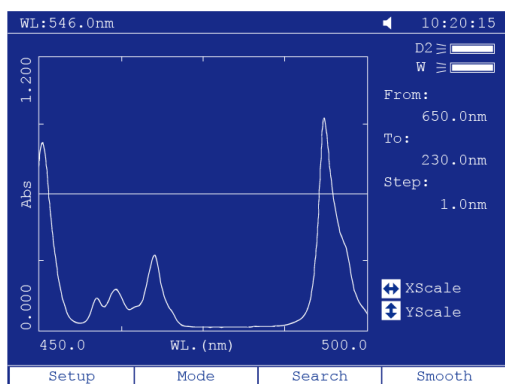

The spectrum scan will then be shown with the updated range values.

To return to the full spectrum scan the user will need to re-enter the original wavelength and photometric range values.


7.6 SPECTRUM SEARCH

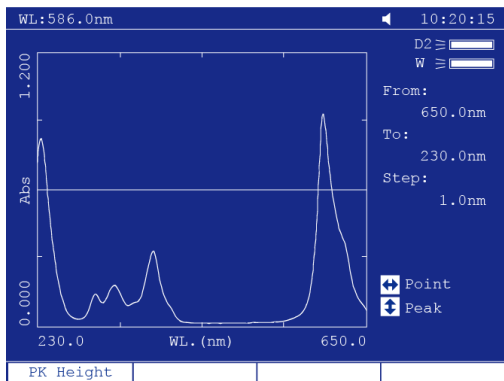

The photometric values of the measured spectrum can be viewed by pressing the function key below the Search option. The user can press the up and down arrow keys to move between the peaks in the scan that are above the threshold peak height. The user can alternatively press the left or right arrow keys to review each point in the scan in turn.


The peak height threshold can be adjusted by pressing the function key below the PK Height option. The threshold peak height value can be entered using the numeric keypad. Press the Enter key to confirm.

7.7 SPECTRUM SMOOTHING

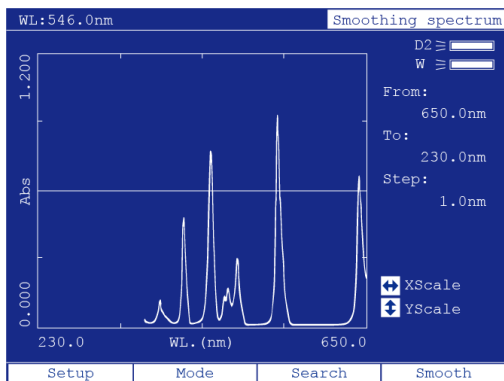

The measured spectrum scan can be smoothed by pressing the function key below the Smooth option.


7.8 STORING RESULTS

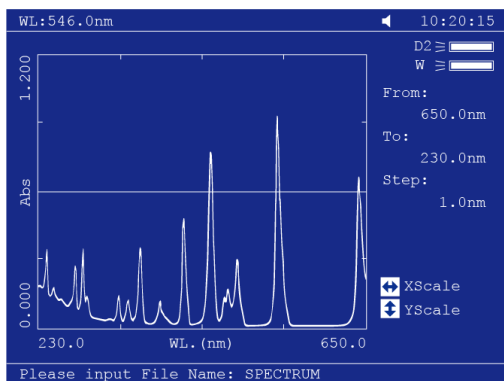

A result file can be saved to the instrument's internal memory.

Press the Save key on the instrument keypad. The instrument will ask the user to enter a filename (max. 8 characters) using the alpha-numeric keypad. The user can select the indicated letters, numbers and symbols by repeatedly pressing the key until the required value is displayed, after a short period the next character can be entered in the same manner. Once the filename has been entered, press the Enter key to confirm.

7.9 RECALLING STORED RESULTS

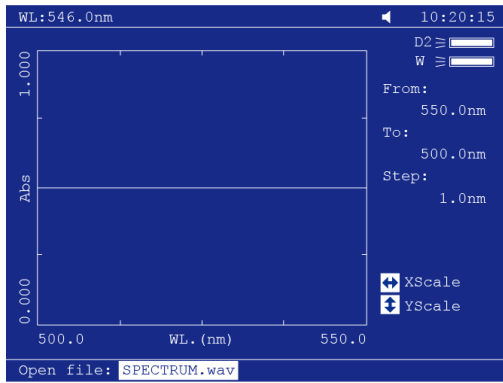


A result file can be opened from the instrument's internal memory.

Press the Open key on the instrument keypad. The user can select from the list of stored files by pressing the up and down arrow keys. Once the required file has been located press the Enter key to confirm.

SECTION 8 – KINETICS

The kinetics measurement mode enables the absorbance or % transmittance of an active molecule to be measured over a period of time; for example enzyme analysis of horseradish peroxidase. The absorbance or % transmittance is measured at regular time intervals at a set wavelength over a period of time. The results are plotted on a graph to show the change in absorbance or % transmittance over time. Following sample measurement statistical analysis of all or part of the experiment can be performed.

8.1 KINETICS MODE SCREEN

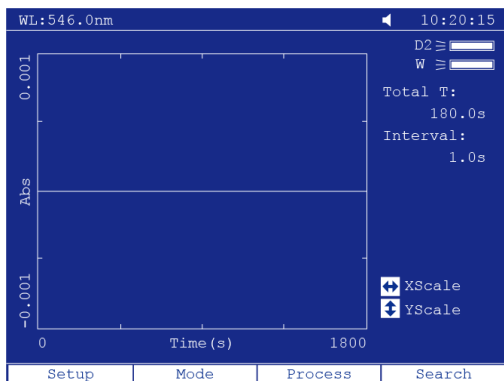


Operating Menu

The kinetics measurement mode enables measurement parameters to be changed and post measurement tools to be accessed. The four options at the bottom of the screen allow the user to edit the kinetics run settings, select the measurement mode, perform a linear regression analysis on the data and perform a post measurement search of the scan's data points. These options are selected with the corresponding function buttons.

8.2 WAVELENGTH SELECTION

The wavelength can be adjusted by pressing the GOTO λ key on the instrument keypad. The required wavelength can then be entered using the numerical keypad. Press the Enter key to confirm.

8.3 METHOD SETUP

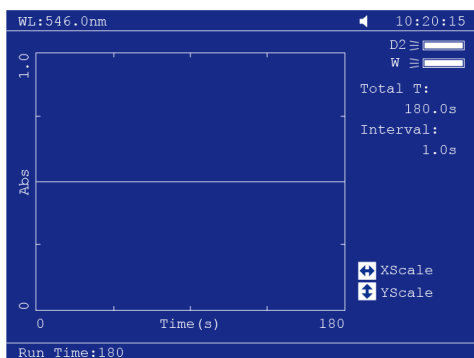

The kinetics scan settings can be edited by pressing the function key below the Setup option. The options that can be changed are:-


1. Run Time
2. Delay Time
3. Time Interval

The numeric keypad should be used to enter the required run and delay times and the up and down arrow keys are used to select from the available time interval options. Press the Enter key to confirm.

8.3.1 Selecting the Measurement Mode


The measurement mode can be selected by pressing the function key below the Mode option. The required measurement mode can then be selected from the available options of Abs and %T using the up and down arrow keys. Press the Enter key to confirm.

8.4 SAMPLE MEASUREMENTS

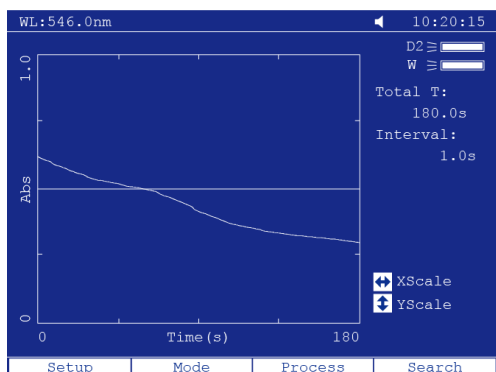


Insert a cuvette containing the blank solution into the reference position in the sample chamber and insert the cuvette containing the sample solution into the sample position. Close the instrument lid and press the Start/Stop key on the keypad. Once the measurement is complete the measured kinetics scan will be displayed on the screen.

8.5 ADJUSTING THE DISPLAYED SCAN RANGE

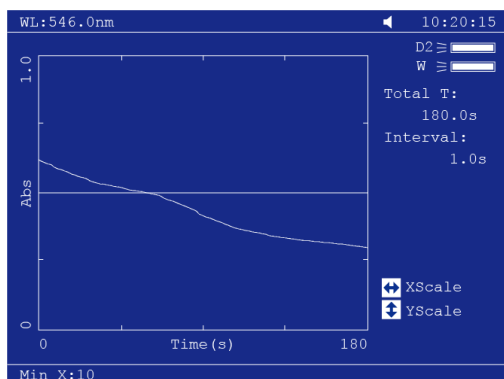


The instrument will display the full range scan after a measurement is complete. To change the displayed time range, press the left or right arrow keys. The start and end times can be entered using the numeric keypad. Press the Enter key to confirm. To change the displayed photometric range, press the up or down arrow keys. The minimum and maximum values can be entered using the numeric keypad. Press the Enter key to confirm.

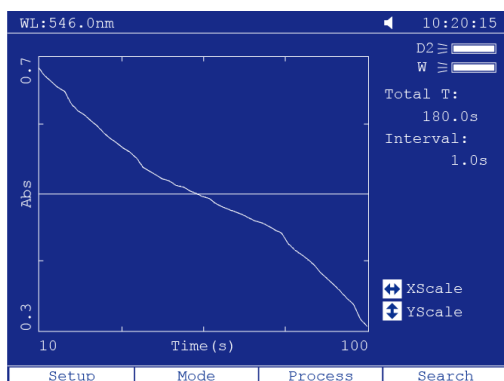

The kinetics scan will then be shown with the updated range values.


The return to the full kinetics scan the user will need to re-enter the original time and photometric range values.

8.6 CALCULATING I/U CONCENTRATION

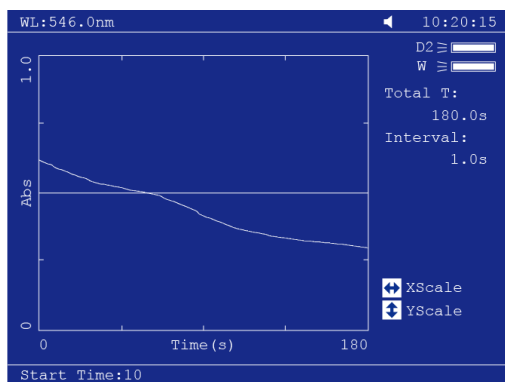

The instrument software allows the user to calculate the concentration of a substance from the difference between the photometric values at two time points in the displayed kinetics scan.

To enter the calculation parameters press the function key below the Process option and enter a Start Time, an End Time and a Factor, pressing the Enter key to confirm each value.

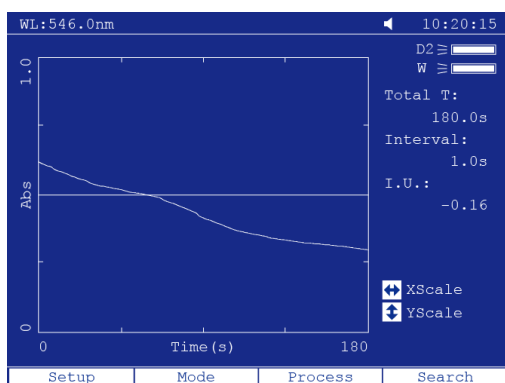


When all values have been confirmed the instrument will calculate the concentration value according to the following equation:

$$\text{Conc (I/U)} = [\text{Abs}_{(\text{start time})} - \text{Abs}_{(\text{end time})}] \times \text{Factor}$$


The calculated concentration value will be displayed on the kinetics mode screen.

8.7 SPECTRUM SMOOTHING

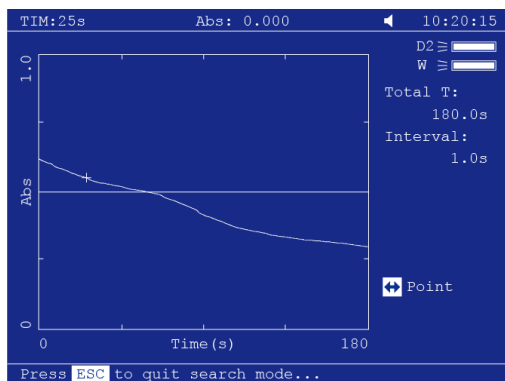

The photometric values of the measured kinetics scan can be viewed by pressing the function key below the Search option. The user can press the up and down arrow keys to review each point in the scan in turn.


8.8 STORING RESULTS

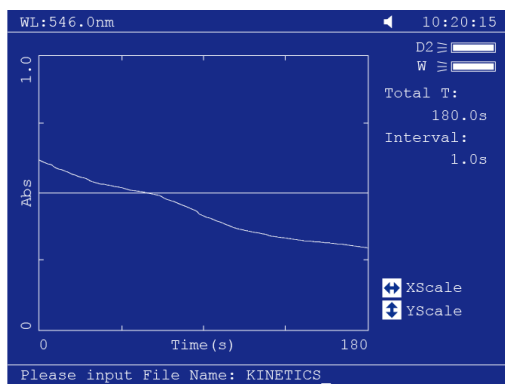

A result file can be saved to the instrument's internal memory.

Press the Save key on the instrument keypad. The instrument will ask the user to enter a filename (max. 8 characters) using the alpha-numeric keypad. The user can select the indicated letters, numbers and symbols by repeatedly pressing the key until the required value is displayed, after a short period the next character can be entered in the same manner. Once the filename has been entered, press the Enter key to confirm.

8.9 RECALLING STORED RESULTS

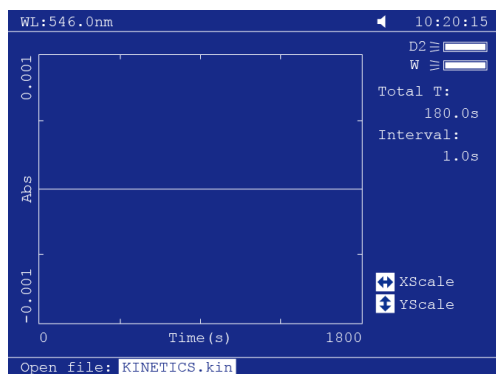


A result file can be opened from the instrument's internal memory.

Press the Open key on the instrument keypad. The user can select from the list of stored files by pressing the up and down arrow keys. Once the required file has been located press the Enter key to confirm.

SECTION 9 – DNA/PROTEIN


The DNA/Protein measurement mode allows the user to measure multi-wavelength absorbance ratios, such as 260nm/280nm and 260nm/230nm, which are commonly used to estimate a protein or nucleic acid sample's purity. The mode also includes calculations that can be used to estimate the concentration of the protein or nucleic acid sample.

9.1 DNA MENU OPTIONS

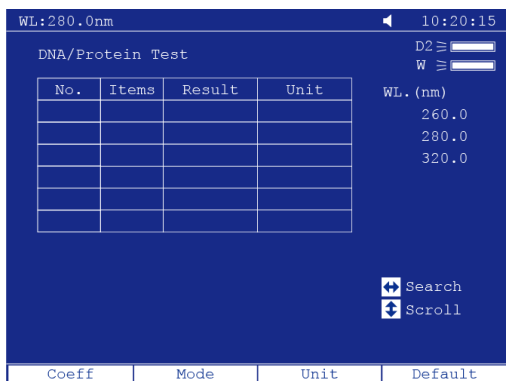

The DNA/Protein measurement mode enables measurement parameters to be changed. The four options at the bottom of the screen allow the user to edit the concentration calculation factors, select the measurement mode, select the units of the measurement and reset the modes settings to their default values. These options are selected with the corresponding function buttons.

9.2 ADJUSTING THE MEASUREMENT MODE

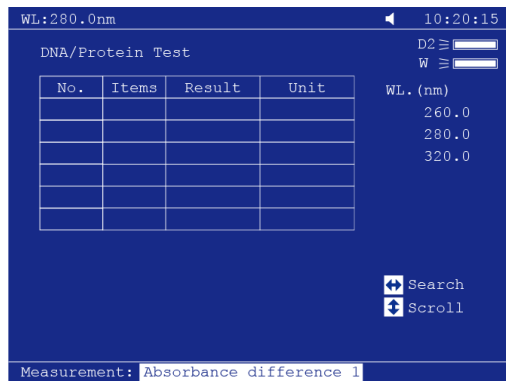

The DNA/Protein measurement mode includes two sets of calculations to calculate the concentration of nucleic acid and protein samples. The measurement mode option can be selected by pressing the function key below the Mode option. The options that are available are:-

1. Absorbance Difference 1
2. Absorbance Difference 2


The default equations and factors used by the instrument are shown below:-

Absorbance Difference 1

$$\text{Purity Ratio} = \text{Abs@260nm} / \text{Abs@280nm}$$

$$\text{DNA Conc } (\mu\text{g/ml}) = (\text{Abs@260} \times 62.9) - (\text{Abs@280} \times 36.0)$$

$$\text{Protein Conc } (\mu\text{g/ml}) = (\text{Abs@280} \times 1553) - (\text{Abs@260} \times 757.3)$$

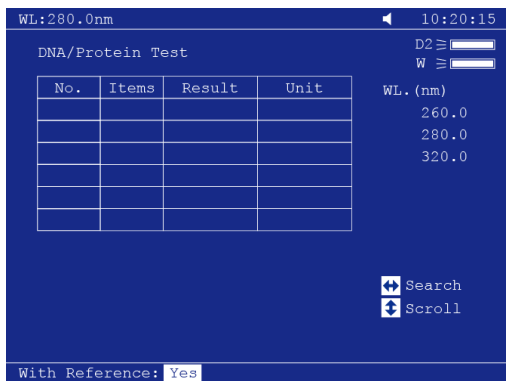

Absorbance Difference 2

$$\text{Purity Ratio} = \text{Abs@260nm} / \text{Abs@230nm}$$

$$\text{RNA Conc } (\mu\text{g/ml}) = (\text{Abs@260} \times 49.1) - (\text{Abs@230} \times 3.48)$$


$$\text{Protein Conc } (\mu\text{g/ml}) = (\text{Abs@230} \times 183) - (\text{Abs@260} \times 75.8)$$

The option to include the third wavelength as a reference is given after the measurement mode is selected. Use the up and down arrow keys to select Yes or No and press the Enter key to confirm. Selecting the Yes option will result in all the absorbance value measured at wavelength 3 being subtracted from the photometric values measured at wavelengths 1 and 2.

9.3 WAVELENGTH SELECTION

The measurement wavelengths of the selected measurement mode can be adjusted by pressing the GOTOλ key on the instrument keypad. The required wavelengths can then be entered using the numerical keypad. Press the Enter key to confirm.

9.4 ADJUSTING THE CONCENTRATION CALCULATION FACTORS

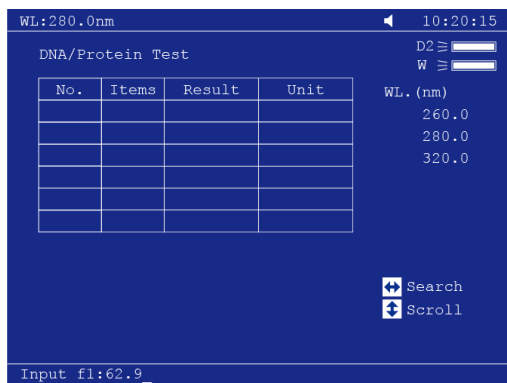

The measurement mode option can be selected by pressing the function key below the Coeff option.

The new concentration calculation factors can be entered using the numeric keypad. Press the Enter key to confirm.

9.5 SELECTING THE UNIT OF MEASUREMENT

The unit of measurement can be selected by pressing the function key below the Unit option. The required unit of measurement can then be selected from the available options of IU, mM/L, M/L, μg/mL, mg/mL, mg/L, mEq, ppb, ppm, % and other. Press the Enter key to confirm.

9.6 RESET MODE SETTINGS

The DNA/Protein mode settings can be reset to their default values by pressing the function key below the Default option.

9.7 DNA/PROTEIN MEASUREMENTS

WL:260.0nm 10:20:15

DNA/Protein Test

No.	Items	Result	Unit
1	A1	0.251	Abs
	A2	0.243	Abs
	Aref	0.095	Abs
	C-DNA	4.524	ug/ul
	C-Pro	110.8	ug/ul
	Ratio	1.059	

WL. (nm)
260.0
280.0
320.0

Search
Scroll

Coeff	Mode	Unit	Default

Ensure that a cuvette containing the blank solution is in the reference position in the sample chamber and insert the cuvette containing the sample solution into the sample position. Close the instrument lid and press the Start/Stop key on the keypad. Once the measurement is complete the determined results will be displayed in the DNA/Protein mode screen. Further samples can be measured in a similar manner.

9.8 STORING METHODS/RESULTS

WL:260.0nm 10:20:15

DNA/Protein Test

No.	Items	Result	Unit
1	A1	0.251	Abs
	A2	0.243	Abs
	Aref	0.095	Abs
	C-DNA	4.524	ug/ul
	C-Pro	110.8	ug/ul
	Ratio	1.059	

WL. (nm)
260.0
280.0
320.0


Search
Scroll

Please input file name:DNA

A method/result file can be saved to the instrument's internal memory.

In the DNA/Protein mode screen press the Save key on the instrument keypad. The instrument will ask the user to enter a filename (max. 8 characters) using the alphanumeric keypad. The user can select the indicated letters, numbers and symbols by repeatedly pressing the key until the required value is displayed, after a short period the next character can be entered in the same manner. Once the filename has been entered, press the Enter key to confirm.

9.9 RECALLING STORED RESULTS

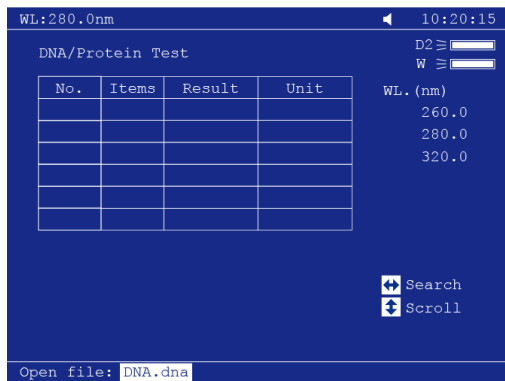

A method/result file can be opened from the instrument's internal memory.


In the DNA/Protein mode screen press the Open key on the instrument keypad. The user can select from the list of stored files by pressing the up and down arrow keys. Once the required file has been located press the Enter key to confirm. If more than one result is stored in a file the up and down arrow keys can be pressed to scroll through the results.

Alternatively the user can press the left or right arrow key to enable a search option. The number of the result that is to be viewed is entered using the numeric keypad. Press the Enter Key to confirm.

SECTION 10 – MULTI-WAVELENGTH


The multi-wavelength measurement mode allows the user to measure a sample's photometric absorbance or %transmittance at up to 10 wavelengths. Following sample measurement, the photometric readings are displayed on the multi-wavelength mode screen.

10.1 MULTI-WAVELENGTH MODE OPTIONS

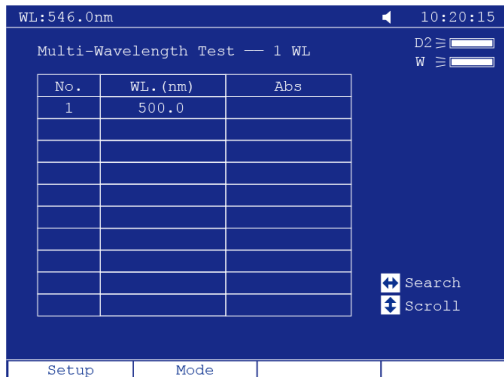


The multi-wavelength measurement mode enables measurement parameters to be changed. The two options at the bottom of the screen allow the user to edit the measurement wavelengths and change the measurement mode. These options are selected with the corresponding function buttons.

10.2 WAVELENGTH SELECTION

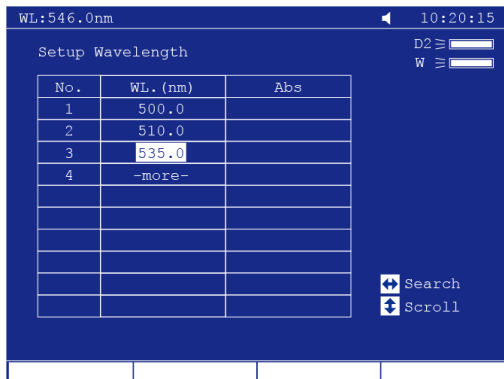


The measurement wavelengths of the selected measurement mode can be adjusted by pressing the function key below the WL Setup option or the GOTOλ key on the instrument keypad. The required wavelengths can be entered using the numerical keypad, pressing the Enter key to confirm each value. Further values can be added by moving to a new line with the down arrow key. Once all the required wavelengths have been entered press the ESC key to exit the wavelength selection screen.

10.3 SAMPLE MEASUREMENT

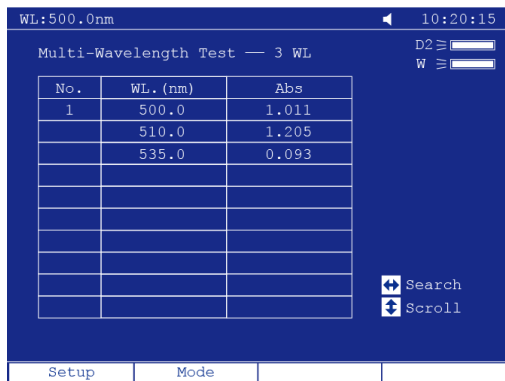

Insert a cuvette containing the sample to be analysed into the sample chamber and press the key below the sample measurement icon. The instrument will take a reading at each of the specified wavelengths the operating menu screen will then display the result of the selected measurement calculation and the photometric readings for each of the measured wavelengths.

10.4 STORING METHODS/RESULTS

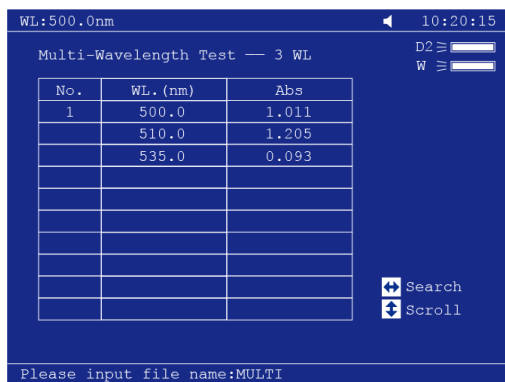


A method/result file can be saved to the instrument's internal memory.

In the multi-wavelength mode screen press the Save key on the instrument keypad. The instrument will ask the user to enter a filename (max. 8 characters) using the alpha-numeric keypad. The user can select the indicated letters, numbers and symbols by repeatedly pressing the key until the required value is displayed, after a short period the next character can be entered

in the same manner. Once the filename has been entered, press the Enter key to confirm.

10.5 RECALLING STORED RESULTS

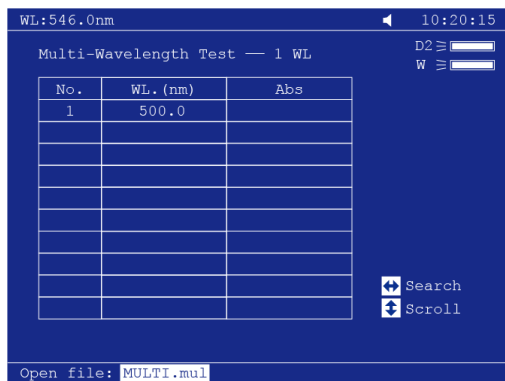


A method/result file can be opened from the instrument's internal memory.

In the multi-wavelength mode screen press the Open key on the instrument keypad. The user can select from the list of stored files by pressing the up and down arrow keys. Once the required file has been located press the Enter key to confirm. If more than one result is stored in a file the up and down arrow keys can be pressed to scroll through the results.

Alternatively the user can press the left or right arrow key to enable a search option. The number of the result that is to be viewed is entered using the numeric keypad. Press the Enter Key to confirm.

SECTION 11 – SAVING/RECALLING RESULTS USING A USB MEMORY STICK

There is a USB port on the side of the instrument for data storage.

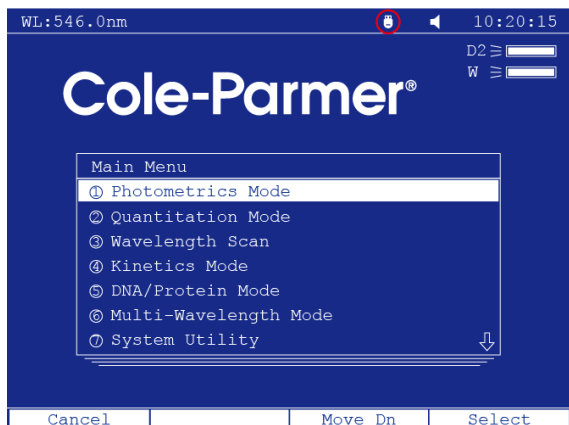

The instrument only recognises a USB memory stick being inserted or removed when it is operating in the home screen. A USB icon appears at the top of the home screen (circled in red).

Insert the USB memory stick when the instrument is in the home screen and enter the required measurement mode. Perform the measurement or measure the standards (Quantitation mode) and press the SAVE button. Enter the file name required using multiple presses of the numeric keys to select the required letter. Press Enter to confirm the file name and the result is saved to the USB memory stick.

Please note that in the Photometrics measurement mode the readout is live; therefore results can't be saved to the internal memory of the instrument or to USB memory stick. In the Quantitation measurement mode it is possible to save the data used to create the calibration curve and to save results to USB memory stick. In the Spectrum, Kinetics, Multi-wavelength and DNA/Protein measurement modes it is possible to save results to USB memory stick.

To open results from the USB memory stick on the instrument insert the USB memory stick when the instrument is in the home screen and enter the required measurement mode. Press the OPEN button and scroll through the saved file names to the required result. Press Enter and the result will open on the screen.

To open results from the USB memory stick in the PC software (Prism) select the corresponding measurement mode in the PC software. From the File drop down menu select Open, select the location of the USB stick memory stick and select the required result.

SECTION 12 – ACCESSORIES AND SPARE PARTS

12.1 OPTIONAL ACCESSORIES


Order Code	Part Code	Description of Accessory
83070-53	685 204	10 x 10mm path length cuvette holder
83070-55	685 131	Water heated 10 x 10mm single cuvette holder
83070-57	685 005	10 to 100mm adjustable path length cuvette holder
83070-59	685 304	Micro-cuvette holder
83070-61	685 401	8 position automatic cell changer
83065-67	035 091	UV/Visible calibration set
99610-35	060 422	Moulded cuvette rack for 16 10x10mm cuvettes
83070-38	035 143	Pack of 100 disposable micro-cuvettes (70µl)
83070-74	685 035	Prism PC software CD and security dongle
83070-75	685 040	Dust cover

12.2 INSTALLING THE PASSIVE AND ACTIVE ACCESSORIES

There are two types of accessories which can be fitted in the sample chamber – passive or active accessories. The range of passive accessories includes 10 x 10mm cuvette holders, water heated cuvette holders, adjustable path length (10 to 100 mm) cuvette holders and micro-cuvette holders. The active accessory is an 8 position automatic cell changer. The instrument must be turned off before any accessories are fitted.

12.2.1 Passive Accessories

Fixing
screws

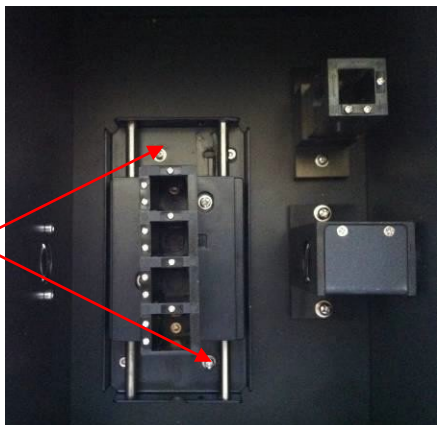


Unscrew the two fixing screws to undo the passive accessory. Lift out the passive accessory. To fit a different passive accessory place the accessory in the correct orientation and re-tighten the two fixing screws to fix in place.

To replace the passive accessory with an active accessory refer to section 11.2.2.

12.2.2 Active Accessories

12.2.2.1 8 Position Automatic Cell Changer

Fixing
screws

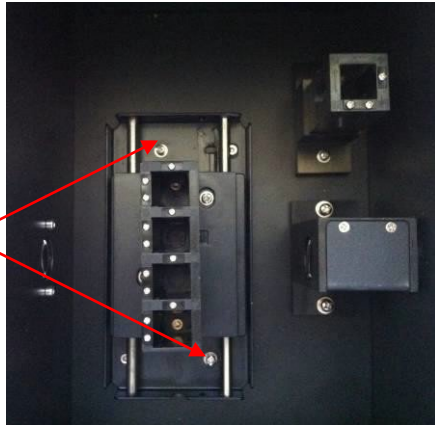

Unscrew the two fixing screws to undo the passive accessory. Lift out the passive accessory.

Accessory
connector




On the underside of the 8 cell accessory, locate the accessories power supply and communication connector.



Take the 8 cell accessory and align the accessories connector with the instrument connection socket.

Fixing screws

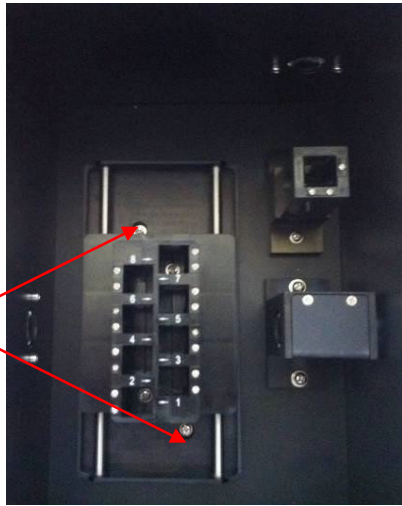


Place the accessory in the correct orientation and re-tighten the two fixing screws to fix the 8 cell accessory in place.

12.3 USING THE 8 POSITION AUTOMATIC CELL CHANGER



When the automatic 8 cell turret is installed the current cell position is indicated below the lamp status icons in the top right hand corner of the screen.

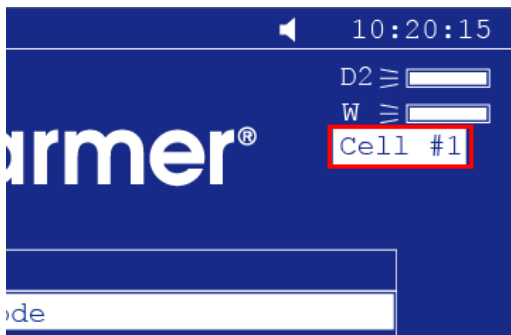

To activate the accessory press the Cell key on the instrument keypad. The indicated cell position will be highlighted on screen.



Each cell position is selected by pressing the corresponding digit on the numeric keypad. e.g. position 6 is selected by pressing the number 6 key on the instrument keypad. The instrument display will update to show the new automatic cell changer position.

Press the Cell key on the keypad to de-activate the 8 position automatic cell changer.

12.4 SPARES

Order Code	Part Code	Description of Spare Part
99956-15	685 020	Tungsten lamp
99956-16	685 021	Deuterium lamp

SECTION 13 – MAINTENANCE AND SERVICE

13.1 ROUTINE MAINTENANCE

Ensure the external surfaces of the unit are clean and free from dust. The sample area should always be kept clean and any accidental spillage should be wiped away immediately. To give added protection when not in use, the unit should be disconnected from the mains supply and covered with the optional dust cover.

13.2 LAMP REPLACEMENT

Warning! HOT.




Switch off the mains power supply and wait at least 20 minutes before attempting to replace the tungsten or deuterium lamps.


13.2.1 Tungsten Lamp Replacement




1. Unscrew the 4 screws indicated (2 screws on each side) and remove the cover of the spectrophotometer.

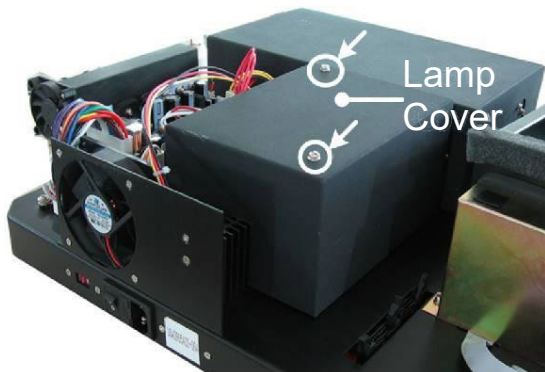

2. Unscrew the 2 screws on the top of the lamp chamber and remove the cover.

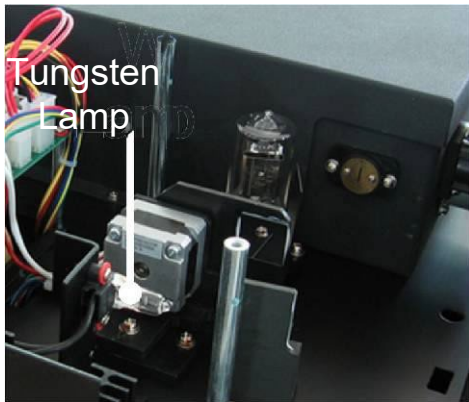

Entrance Window

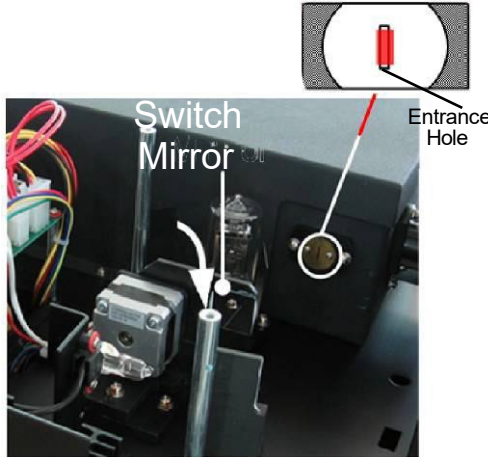


3. Whilst wearing cotton gloves remove the defective tungsten lamp and replace with a new one.

4. Switch on the power and move the Switch Mirror down into the position shown in the picture opposite. Observing the entrance window on the instrument's monochromator, adjust the tungsten lamp until the light is centred on the entrance hole.

5. Disconnect the power and re-attach the lamp compartment cover and the top case of the spectrophotometer.

13.2.2 Deuterium Lamp Replacement

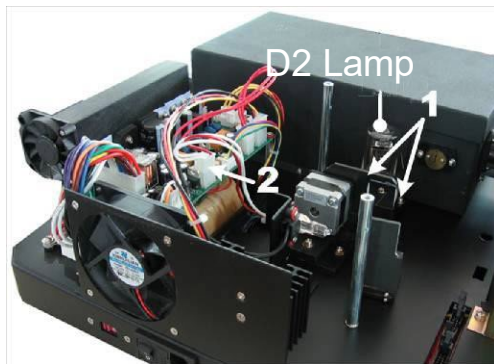

1. Unscrew the 4 screws on the spectrophotometer's top case (see 12.2.1) and remove the cover of the spectrophotometer.

2. Unscrew the 2 screws on the top of the lamp chamber and remove the cover. (see 12.2.1)

3. Unscrew the 2 screws on the deuterium lamp flange (No.1), unplug the connector on the power board (No. 2) and remove the deuterium lamp. Whilst wearing cotton gloves replace with a new deuterium lamp. Re-fix the 2 screws and reconnect the power cable.

4. Re-attach the lamp compartment cover and the top case of the spectrophotometer.

13.3 SERVICE

Our dedicated service team are on hand to help in the unlikely event that your Cole-Parmer equipment develops a fault. Please contact them by one of the following means with a clear description of the problem:

E-mail: cpSERVICE@antylia.com

Tel: +44 (0) 1785 810475

Fax: +44 (0) 1785 810471

On occasion it may be necessary for your equipment to be sent back to our Service Department for repair. In this case please contact the Service Department for a reference number which you should include with your faulty equipment. Please also ensure you include a clear description of the fault and a completed copy of our Decontamination Certificate. This is available as a downloadable pdf file at www.coleparmer.com, or contact us and we will be happy to fax you a copy. Please clearly mark the package for the attention of the Service Department and post to the following address:

Antylia Scientific Ltd
Beacon Road Stone
Staffordshire ST15
0SA
United Kingdom

All replacement parts are guaranteed for 1 year and where ever possible, returned equipment is turned around in 10 working days.

SECTION 14 – TROUBLESHOOTING

14.1 TROUBLESHOOTING GUIDE

Issue	Solution
Unable to achieve a reading when measuring a sample	Ensure the correct cuvettes are being used so that light isn't being absorbed by the cuvette. Ensure the sample isn't too dense that light is not transmitted through the sample. Ensure the lamp is working.

14.2 TECHNICAL SUPPORT

Cole-Parmer have a dedicated Technical Support team made up of experienced scientists who are on hand to help with any applications advice and questions you may have about our products and how to use them. If you require any technical or application assistance please contact the team at:

E-mail: cptechsupport@antylia.com.

Phone: +44 (0)1785 810433

Fax: +44 (0)1785 810405

SECTION 15 – DECLARATION OF CONFORMITY



This product meets the applicable CE Directives and UKCA Legislation for radio frequency interference and may be expected not to interfere with, or be sure that other equipment with similar qualifications. We cannot be sure that other equipment used in its vicinity will meet these standards and so we cannot

guarantee interference will not occur in practice. Where there is a possibility that injury or loss might occur if malfunctions due to radio frequency interference, or general advise before use, contact the manufacturer

Declaration of Conformity is available to view online at www.coleparmer.com

EU Representative address

Cole-Parmer Ltd
Bâtiment le Delta Parc Icade
Paris Nord 2
7 rue du Canal
BP 55437 Villepinte
95944 ROISSY Charles de
Gaulle
France
Tel: +33 (0) 1 48 63 78 00
Email: frsales@antylia.com

UK Representative address

Antylia Scientific
9 Orion Court
Ambuscade Road Colmworth
Business Park St. Neots
PE19 8YX
United Kingdom
Tel: +44 (0) 1480 277339
Email: enquiries@antylia.com

Ordering Information

Order No.	Series	Model	Legacy SKU
83070-04	SP-800	SP-800-UV-115	6850/115V
83070-06	SP-800	SP-800-UV	6850/230V

Warranty Registration



UK

T: +44 (0) 1480 272270
E: uk.sales@antylia.com
W: coleparmer.com

Germany

T: +49 (0) 9377 92030
E: de.sales@antylia.com
W: coleparmer.de

France

T: +33 (0) 1486 37800
E: fr.sales@antylia.com
W: coleparmer.fr

Italy

T: +39 (0) 284349215
E: it.sales@antylia.com
W: coleparmer.com

India

T: +9122 61394444
E: info@coleparmer.in
W: coleparmer.in

China

T: +1 847 549 7600
E: sales@antylia.com
W: coleparmer.com

USA

T: +1 847 549 7600
E: sales@antylia.com
W: coleparmer.com

Canada

T: +514 355 6100
E: info@antylia.ca
W: coleparmer.ca

Other

T: +1 847 549 7600

Cole-Parmer®

Antylia Scientific
Beacon Road
Stone
Staffordshire
ST15 0SA
United Kingdom

