


MicroPette Plus

Fully Autoclavable Mechanical Pipette

The MicroPette Plus pipette is fully autoclavable, being able to withstand temperatures of 121°C and pressure of 1ATM, and does not need to be pre-treated prior. Following the autoclave cycle, a 12 hour cooling and drying period ensures that the high performance of the MicroPette Plus is retained. It is recommended the piston and rubber seals be greased after every 10 cycles of autoclaving.

121°C
FULLY
 Autoclavable

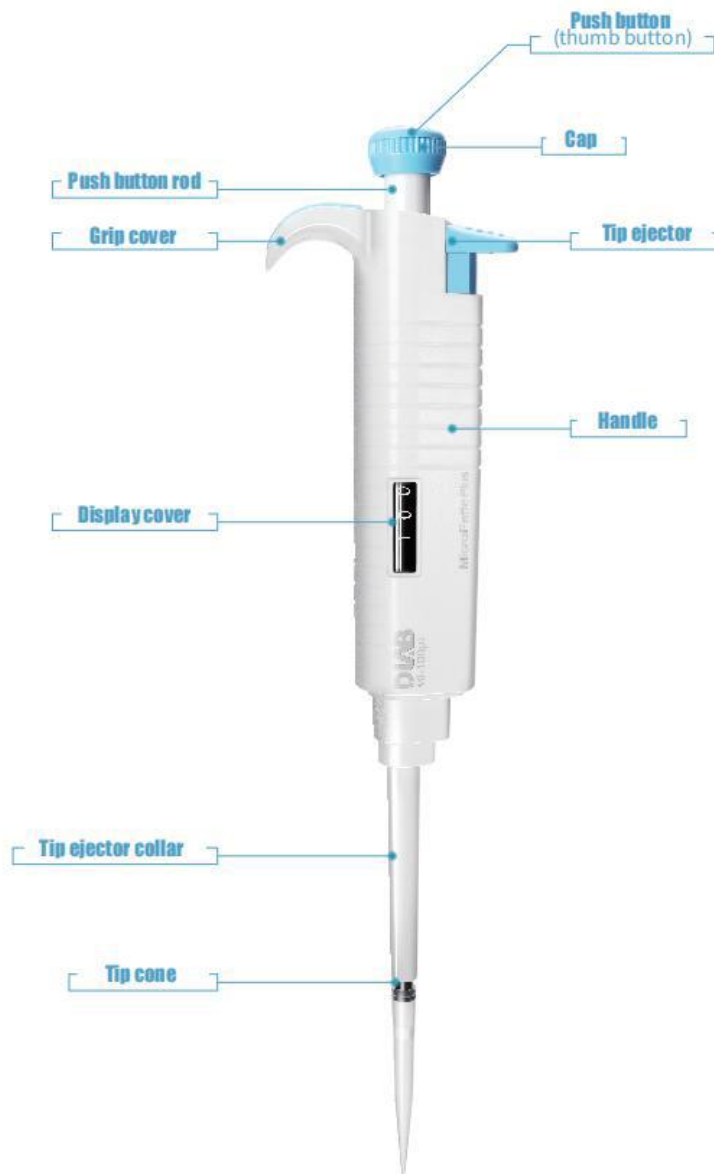

Features

- Available as Fixed Volume and Adjustable Volume formats
- Streamlined shape design
- Comprehensive volume range from 0.1µL to 10mL
- Easy calibration and maintenance
- 8 and 12 channel pipette options
- Dispensing head rotates for effortless pipetting convenience
- Individual piston and tip cone assembly
- Spring loaded tip cones for easy cleaning and maintenance
- Compound material-made tip cone secures high sealing performance



Mechanical Pipette Volume Selection

Specifications

This volume list is for MicroPette and MicroPette plus (Adjustable and Fixed volume)

Single-channel Adjustable Volume Pipettes						
Volume Range	Increment	Test Volume	Error limits in accordance with ISO8655-2			
			Systematic Error		Random Error	
μL	μL	μL	μL	%	μL	%
0.1-2.5	0.05	2.5	± 0.0625	± 2.50	± 0.05	± 2.00
		1.25	± 0.0375	± 3.00	± 0.0375	± 3.00
		0.25	± 0.03	± 12.00	± 0.015	± 6.00
0.5-10	0.1	10	± 0.1	± 1.00	± 0.08	± 0.80
		5	± 0.075	± 1.50	± 0.075	± 1.50
		1	± 0.025	± 2.50	± 0.015	± 1.50
2-20	0.5	20	± 0.18	± 0.90	± 0.08	± 0.04
		10	± 0.12	± 1.20	± 0.1	± 1.00
		2	± 0.06	± 3.00	± 0.04	± 2.00
5-50	0.5	50	± 0.3	± 0.60	± 0.15	± 0.30
		25	± 0.225	± 0.90	± 0.15	± 0.60
		5	± 0.1	± 2.00	± 0.1	± 2.00
10-100	1	100	± 0.8	± 0.80	± 0.15	± 0.15
		50	± 0.5	± 1.00	± 0.2	± 0.40
		10	± 0.3	± 3.00	± 0.15	± 1.50
20-200	1	200	± 1.2	± 0.60	± 0.3	± 0.15
		100	± 0.8	± 0.80	± 0.3	± 0.30
		20	± 0.6	± 3.00	± 0.2	± 1.00
50-200	1	200	± 1.2	± 0.60	± 0.3	± 0.15
		100	± 0.8	± 0.80	± 0.3	± 0.30
		50	± 0.5	± 1.00	± 0.2	± 0.40
100-1000	5	1000	± 6	± 0.60	± 2	± 0.20
		500	± 3.5	± 0.70	± 1.25	± 0.25
		100	± 2	± 2.00	± 0.7	± 0.70
200-1000	5	1000	± 6	± 0.60	± 2	± 0.20
		500	± 3.5	± 0.70	± 1.25	± 0.25
		200	± 1.8	± 0.90	± 0.6	± 0.30
1000-5000	50	5000	± 25	± 0.50	± 7.5	± 0.15
		2500	± 15	± 0.60	± 7.5	± 0.30
		1000	± 7	± 0.70	± 3	± 0.30
2000-10000 Do not apply to MicroPette plus	100	10000	± 60	± 0.60	± 20	± 0.20
		5000	± 60	± 1.20	± 15	± 0.30
		2000	± 60	± 3.00	± 12	± 0.60

User calibration should refer to the industrial standard ISO8655-2.

Fixed Volume Pipettes

Volume Range	Increment	Test Volume	Systematic Error		Random Error	
μL	–	μL	μL	%	μL	%
5	–	5	± 0.065	± 1.3	± 0.06	± 1.2
10	–	10	± 0.08	± 0.8	± 0.08	± 0.8
20	–	20	± 0.12	± 0.6	± 0.1	± 0.5
25	–	25	± 0.125	± 0.5	± 0.075	± 0.3
50	–	50	± 0.25	± 0.5	± 0.15	± 0.3
100	–	100	± 0.5	± 0.5	± 0.3	± 0.3
200	–	200	± 0.8	± 0.4	± 0.4	± 0.2
250	–	250	± 1.0	± 0.4	± 0.5	± 0.2
500	–	500	± 1.5	± 0.3	± 1.0	± 0.2
1000	–	1000	± 3.0	± 0.3	± 2.0	± 0.2
2000	–	2000	± 6.0	± 0.3	± 3.0	± 0.15
5000	–	5000	± 15	± 0.3	± 7.5	± 0.15

8-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Systematic Error		Random Error	
μL	μL	μL	μL	%	μL	%
0.5-10	0.1	10	± 0.15	± 1.50	± 0.15	± 1.50
		5	± 0.125	± 2.50	± 0.125	± 2.50
		1	± 0.04	± 4.00	± 0.04	± 4.00
5-50	0.5	50	± 0.5	± 1.00	± 0.25	± 0.50
		25	± 0.375	± 1.50	± 0.25	± 1.00
		5	± 0.15	± 3.00	± 0.1	± 2.00
10-100	1	100	± 0.8	± 0.80	± 0.3	± 0.30
		50	± 0.5	± 1.00	± 0.4	± 0.80
		10	± 0.3	± 3.00	± 0.2	± 2.00
50-300	5	300	± 2.1	± 0.70	± 0.75	± 0.25
		150	± 1.5	± 1.00	± 0.75	± 0.50
		50	± 0.75	± 1.50	± 0.4	± 0.80
100-1000	10	1000	± 10	± 1.00	± 3	± 0.30
		500	± 10	± 2.00	± 2.5	± 0.50
		100	± 5	± 5.00	± 1	± 1.00

12-channel Adjustable Volume Pipettes

Volume Range	Increment	Test Volume	Systematic Error		Random Error	
μL	μL	μL	μL	%	μL	%
0.5-10	0.1	10	± 0.15	± 1.50	± 0.15	± 1.50
		5	± 0.125	± 2.50	± 0.125	± 2.50
		1	± 0.04	± 4.00	± 0.04	± 4.00
5-50	0.5	50	± 0.5	± 1.00	± 0.25	± 0.50
		25	± 0.375	± 1.50	± 0.25	± 1.00
		5	± 0.15	± 3.00	± 0.1	± 2.00
10-100	1	100	± 0.8	± 0.80	± 0.3	± 0.30
		50	± 0.5	± 1.00	± 0.4	± 0.80
		10	± 0.3	± 3.00	± 0.2	± 2.00
50-300	5	300	± 2.1	± 0.70	± 0.75	± 0.25
		150	± 1.5	± 1.00	± 0.75	± 0.50
		50	± 0.75	± 1.50	± 0.4	± 0.80

* DLAB specifications are used as guidelines and the user calibration should refer to the industrial standard ISO 8655



WolfLabs

Pricing on any accessories shown can be found by keying the part number into the search box on our website.

The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed to be correct. If there are aspects of the specification that must be guaranteed, please provide these to our sales team so that details can be confirmed.

www.wolflabs.co.uk

Tel : 01759 301142

Fax : 01759 301143

sales@wolflabs.co.uk

Please contact us if this literature doesn't answer all your questions.