



HI6221

Advanced pH and ORP Benchtop Meter

Dear Customer,

Thank you for choosing a Hanna Instruments® product.

Please read this instruction manual carefully before using this instrument as it provides the necessary information for correct use of this instrument, as well as a precise idea of its versatility.

If you need additional technical information, do not hesitate to e-mail us at tech@hannainst.com.

Visit www.hannainst.com for more information about Hanna Instruments and our products.

TABLE OF CONTENTS

1. Preliminary Examination	3	9.2. Reading	38
2. Safety Measures	3	9.3. Temperature	39
3. User Interface— Icons	4	9.4. View	41
4. General Description & Intended Use	6	9.5. Alarms	43
4.1. Main Features	7	9.6. Logging	44
5. Specifications	8	9.7. Profiles	46
5.1. Instrument	8	10. Calibration procedure	47
5.2. Electrodes	10	10.1. pH Calibration	48
6. Functional & LCD Description	11	10.2. Relative mV Calibration	52
6.1. Main Unit	11	11. Measurement	53
6.2. Electrodes	13	11.1. Measurement Tips	53
7. Getting Started	14	11.2. Direct Readings	54
7.1. Attaching the Electrode arm	14	11.3. Direct / Autohold Readings	54
7.2. Using the Electrode Holder	15	12. Logging	55
7.3. Connecting Electrodes & Keyboard	15	12.1. Automatic Logging	56
7.4. Powering the Unit, Selecting Operating Language & Regional Preferences	16	12.2. Manual Logging	56
7.5. Basic Operations	17	12.3. Autohold Logging	57
8. System Menu Items	17	13. Maintenance & Conditioning	57
8.1. Users	18	14. Error Messages	59
8.2. System Settings	21	15. Accessories	60
8.3. Measurement Settings	26	16. Abbreviations	66
8.4. Log Recall	29	Certification	67
8.5. Help	35	Recommendations for Users	67
9. Measurement & Electrode Setup Menu	36	Warranty	67
9.1. Calibration	36	Regulatory notices for the Wi-Fi Module	68

All rights are reserved. Reproduction in whole or in part is prohibited without the written consent of the copyright owner, Hanna Instruments Inc., Woonsocket, Rhode Island, 02895, USA. Hanna Instruments reserves the right to modify the design, construction, or appearance of its products without advance notice.

1. PRELIMINARY EXAMINATION

HI6221 is Hanna's® advanced benchtop pH and ORP meter with a large touch screen display and streamlined design. Each HI6221 is supplied with:

- HI1131B pH electrode
- HI7662-TW temperature probe
- pH calibration starter kit consisting of:
 - pH 4.01 buffer solution (2 sachets)
 - pH 7.01 buffer solution sachet (4 sachets)
 - pH 10.01 buffer solution sachet (2 sachets)
- HI700601 electrode cleaning solution sachet (2 sachets)
- HI70300S storage solution for pH & ORP electrodes (25 mL)
- HI7082 3.5M KCl electrolyte solution (30 mL)
- HI764060 electrode holder with following accessories:
 - base plate (with integrated pivot pin) and screw (requires installation)
 - cable holder clip, attached
 - electrode holder with adapter, attached
- Capillary pipette
- 24 VDC power adapter
- USB-C to USB-A cable
- Probe quality certificate
- Quick reference guide with instrument quality certificate

For ORP (redox) measurements a separate sensor is required. See Accessories section for available ORP models.

Note: Save all packing material until you are sure the instrument works correctly. Any damaged or defective item must be returned in its original packing material with the supplied accessories.




2. SAFETY MEASURES






Handling and usage precautions






The unit, while not fragile, can be damaged by improper handling and usage.







- Transport the unit with all cables removed.
- Keep the unit on a stable and even surface, away from contact with liquid.
- Avoid excessive dirt and dust.
- Protect the unit from contact with food, oils, and chemicals.
- If the device becomes wet, gently wipe the exterior with a clean, dry cloth.
- Keep away from direct sunlight.
- Use in a safe place that is appropriate to application requirements.
- Use attachments and accessories specified in this manual only.
- Capacitive touchscreen and buttons — operate without applying pressure.
- Do not puncture the capacitive touchscreen or drop the unit.
- Do not use the device near heat sources.
- Do not place objects on top of the device.
- Do not insert objects into the ports, spaces around keys, other than the intended cable, USB drive.

3. USER INTERFACE – ICONS

Capacitive keys	Description
	Back – return to a previous hierarchical menu level
	Home – access to measurement screen & configured profile
	Menu – access to Users, System Settings, Measurement Settings, Log Recall, Help

Main menu	Description
	Users – login & rights configuration
	System Settings – system configuration, connectivity & printing items
	Measurement Settings
	Log Recall – access logged measurement data
	Help – access support

Measurement	Description
	Measurement Menu, accessed from measurement screen
	pH electrode (seen in full GLP view)
	Autohold applied
	Autohold, waiting stable pH/mV measurement
	Warning on standby/ active function

Logging	Description
	Start/ Stop logging (current index and time since log start)
	Manual logging (current index)
	Triggers log session, pending next stable measurement
	Autohold logging in progress
	Annotated text/Annotated text in use
	Available storage capacity (at full capacity the icon is displayed blinking)

Log recall


Description



Table view, function active/not selected



Graph view, function active/not selected



Information view, function active/not selected

General

Description



Profile



Background operation in progress



Alarm enabled



Stability/Autohold indicator

Active buffer selection during manual or semiautomatic calibration
Forward/backward navigation, sequence of steps
(gray icon: function not available)Calibration procedure, buffer selection, tutorial sequence of steps
(gray icon: function not available)

Connectivity & Printing

Description

Ethernet



Connection established (tap for IP address)



0.5 sec.



Connection in progress



Connection error

Wi-Fi



Connection established (tap for IP address)



0.5 sec.



Connection in progress



Connection error

USB



USB-A or USB-C key plugged in



High-power consumption with key plugged in

PC



PC connection established through USB-C port

Printer

Printer connected - printing manual log option **enabled**Printer connected - printing manual log option **disabled**

Printer not recognized or no longer connected

4. GENERAL DESCRIPTION & INTENDED USE

HI6221 is an advanced benchtop meter with a capacitive display, comprised of a housing and an integrated pH/ORP measurement module. Compact and easy to operate, the meter is delivered with Hanna Instruments **HI1131B** combination pH electrode and **HI7662-TW** temperature probe for pH measurement.

A separate ORP sensor is required for ORP measurements.

HI1131B is a glass body, double junction, refillable pH electrode with an indicating sensor made of high temperature (HT) glass. The double junction reference and HT glass design allow the **HI1131B** to be used in a wide variety of applications.

Probe connection to the unit is secured through a galvanically isolated BNC connection.

HI7662-TW stainless steel temperature probe allows the meter to perform automatic temperature compensation (ATC).

This system responds to a complex range of measurement and monitoring requirements, providing accuracy, reproducibility, and reliability.

HI6221 is supplied with an electrode holder that has a flexible arm. The holder can be mounted quickly and provides secure support for electrodes while taking measurements in sample containers.

This benchtop meter supports:

- USB type A — support for USB drive, printer, keyboard
- USB type C — support for USB drive, PC connection

The user can select between five different views.

- Basic measurement configuration
- Simple GLP with calibration information
- Full GLP with electrode status and calibration point details (pH only)
- Live updated, interactive graph
- Tabulated data with date, time, and notes

Capacitive touch screen with multi-touch support

The benchtop unit has a 7-inch color display with 800 x 480p resolution. The capacitive, multi-touch screen supports video playback and data plotting.

4.1. MAIN FEATURES

Measurement & Calibration

- Measure pH/mV (pH) or mV/Rel.mV (ORP) with temperature
- Application-specific profiles allow quick and direct measurement without the need to update the sensor and system settings
- Active log during measurement
- Measurement stability indicator (using the Stability Criteria setting)
- Reading modes: direct and direct/autohold
- pH temperature compensation can be Automatic (using temperature probe) or set manually
- Audible and/or alarm messages for measurements outside predefined limits
- Galvanic isolation for pH/ORP measurement module
- 5-point pH calibration with automatic recognition for standard buffers (Hanna and NIST buffers)
- Choice of standard or custom buffers for calibration
- Non-volatile memory saves data and settings

Logging

- Data log collection of at least 1 000 000 data points (with time and date stamp)
- Logging types: manual, automatic, autohold
- Sample ID for manual and autohold data

Connectivity features & services

- Transfer logged data to a USB thumb drive
- Log files include measurements and calibration data (as .CSV file)
- FTP and email for log export via Ethernet and Wi-Fi connection
- Download logs using the benchtop's embedded web server
- USB type A for USB drive, printer, and keyboard
- USB type C for USB drive and PC connection

User-support feature

- Help section — brief overview of instrument's main functionalities and features

5. SPECIFICATIONS

5.1. INSTRUMENT

pH	Range*	-2.0 to 20.0 pH -2.00 to 20.00 pH -2.000 to 20.000 pH
	Resolution	0.1 pH 0.01 pH 0.001 pH
	Accuracy	±0.1 pH ±0.01 pH ±0.002 pH (±1 last significant digit)
mV	Range	-2000.0 mV to 2000.0 mV
	Resolution	1 mV 0.1 mV
	Accuracy	±0.2 mV ±1 last significant digit
Temperature	Range	-20.0 to 120.0 °C -4.0 to 248.0 °F 253.2 to 393.2 K
	Resolution	0.1 °C / 0.1 °F / 0.1 K
	Accuracy	±0.2 °C / ±0.4 °F / ±0.2 K
Relative mV offset	Range	±2000.0 mV
Reading	Modes	Direct Direct/Autohold
	Stability criteria	Accurate Medium Fast
	Isopotential	-2.000 to 20.000 pH
	Sampling rate	1000 ms
	Calibration points	Up to 5
pH calibration	Type	Automatic Semiautomatic Manual
	Standard buffers	Hanna and NIST pH 1.68, 3.00, 4.01, 6.86, 7.01, 9.18, 10.01, 12.45
	Custom buffers	Up to 5
	Custom group	Up to 5
	1 st calibration point	Offset or Points (user setting)
	Reminder	Daily: 0 min. to 23 hours and 59 min. Periodic: 1 min. to 30 days, 23 hours and 59 min. Disabled

*The range may be limited by the probe's limits.

Temperature user calibration		1 point, adjustable
pH views	Basic	Measurement pH: pH measurement and pH mV mV: measurement Rel.mV: measurement, Absolute mV Temperature (ATC or MTC) Measurement profile (when enabled) Stability status
	Simple GLP	Basic view information pH last calibration date, electrode offset, average slope, and electrode condition (for 24 hours after calibration) Rel. mV: Last Calibration, Offset
	Full GLP (pH only)	Simple GLP information and calibration point details
	Graph (Plot)	pH, mV, Rel. mV and temperature versus time graph can be panned or zoomed (pinch-to-zoom technology)
	Table	Measurements updated every second are displayed in table. With Manual logging type, configuration displays table of logged data points.
pH temperature compensation		Automatic or Manual
Logging	Type	Automatic Manual Autohold
	Number of records	50 000 maximum per file Stores at least 1 000 000 data points per user
	Automatic interval	1, 2, 5, 10, 30 seconds 1, 2, 5, 10, 15, 30, 60, 120, 150, 180 minutes
	Sample ID	Incremental mode or manual
	Export option	.CSV file format
Users		Up to 9 users and the default administrator account
Connectivity	USB-A	2 ports for keyboard and/or printer input or USB thumb drive
	USB-C	1 port for PC connectivity and USB-C type thumb drive
	Wi-Fi & Ethernet	FTP Web server Log transfer and download Email
	RS232	Connecting peripherals
Power supply		DC adapter 100-240 VAC to 24 VDC 2 A
Environment		0 - 50 °C / 32 - 122 °F / 273 - 323 K maximum 95 % RH non-condensing
Dimensions		205 x 160 x 77 mm (8.0 x 6.2 x 3.0 ")
Weight		Approximately 1.2 kg (26.5 lbs.)

5.2. ELECTRODES

HI1131B – pH electrode

Range	0 to 13 pH
Reference cell type	Double, Ag/AgCl
Junction type	Ceramic Single 15-20 μ L per h
Refill electrolyte	3.5M KCl
Maximum pressure	0.1 bar
Body material	Glass
Tip shape	Spheric (\emptyset 9.5 mm)
Operating temperature	-5 to 100 °C (23 to 212°F) – HT
Temperature sensor	No
Amplifier	No
Cable	Coaxial; 1 m (3.3')
Recommended use	Laboratory samples, general purpose


HI7662-TW – Temperature probe

Body material	Stainless steel
Connector type	RCA Phono connector
Dimensions	Total length: 100 mm (3.94 ") Active part: \emptyset 3 mm (0.12 ")
Cable	1 m (3.3') length

6. FUNCTIONAL & LCD DESCRIPTION


6.1. MAIN UNIT

Front View

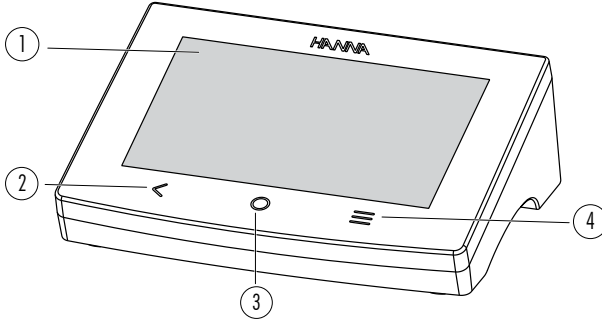

1. LCD display	3. Home key
2. Back key	4. Menu key

LCD Description

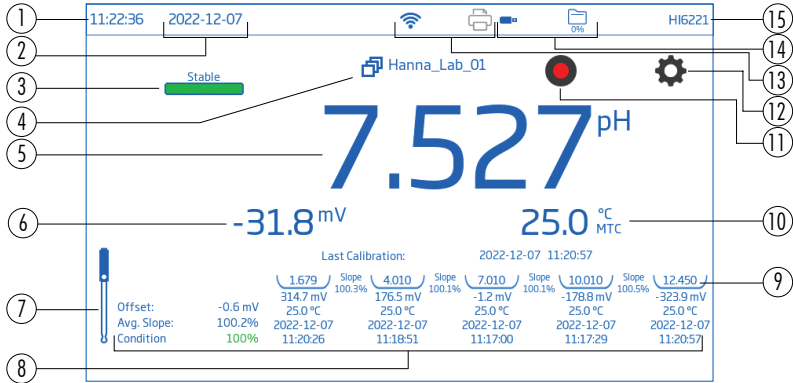

1. Current time	9. Buffer trays
2. Current date	10. Temperature reading and temperature compensation status
3. Stability indicator	11. Start logging icon
4. Measure profile	12. Measurement Menu icon
5. pH reading	13. Connectivity and Printer icons
6. pH mV reading	14. USB connection status and Logging space availability
7. pH electrode icon	15. User name (default "Admin")
8. Calibration information	

Status Area




Continuously displayed after powering the unit, status area runs horizontally across the top of the LCD screen.

- Top left – current time & date
- Middle – connectivity status
- Top right – storage space availability & username

Direct Keys

Icon	Name	Function
<	Back	<ul style="list-style-type: none"> • returns user to previous hierarchical menu level • exit or escape function
○	Home	<ul style="list-style-type: none"> • access to measurement screen • exit or escape function
≡	Menu	<ul style="list-style-type: none"> • access to Users, System Settings, Measurement Settings, Log Recall, Help


Rear View

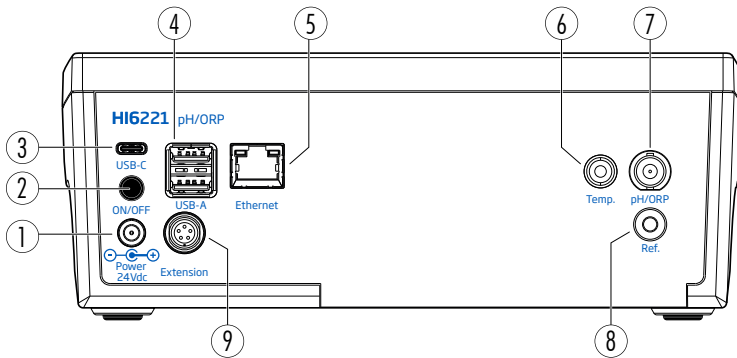

1. Input for power cable
2. Power button
3. Input for USB-C flash or PC cable
4. Input for USB-A flash (x2) or keyboard/printer
5. Ethernet port
6. Temperature probe connection port
7. pH/ORP probe connection port
8. Reference electrode socket
9. Peripherals port


6.2. ELECTRODES

HI1131B
pH electrode

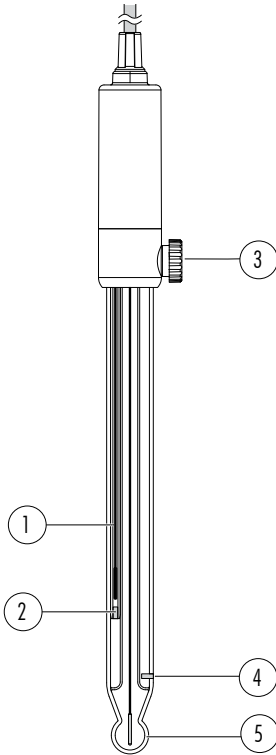

-
1. Reference wire
 2. Inner reference junction
 3. Reference fill cap
 4. Outer reference junction
 5. Glass bulb
-

HI7662-TW
Temperature probe

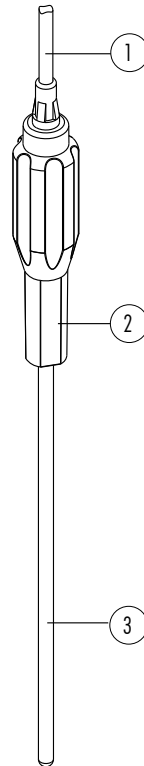


-
1. Cable
 2. Handle
 3. Stainless steel tube
-

7. GETTING STARTED

7.1. ATTACHING THE ELECTRODE ARM

Attaching the electrode holder base plate

- Take the **HI764060** electrode arm from the box.
- Identify the metal base plate (4) with the integrated pivot pin (5) and the screw (2).
- The plate may be attached to either side of the meter, left (L) or right (R).
- Place the meter face down on a clean, dry surface.
- Align the hole on the base plate (3) over the rubber foot (6R or 6L). The pivot pin (5) should be facing downward.
- Use a screwdriver (1) to tighten the screw (2) and attach the base plate to the meter.

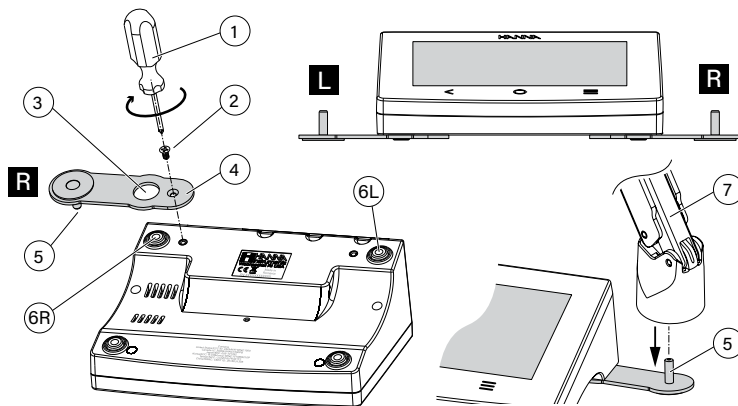


- Position the meter with the display facing up.
- Slide the electrode holder (7) over the pivot pin (5). A “slide in” motion is required to lock the arm into position.
- For increased arm rigidity, tighten the metal knobs on both sides of the electrode arm.

Cable holder clip

The electrode holder is delivered with a cable holder clip (attached) that secures several cables whilst allowing them to move freely with the arm motion.


1. To open the latch, press the clip inward while pulling up the latch.
2. To close the latch, lower latch over cable and snap closed.

The latch snaps in position and secures the cables inside.

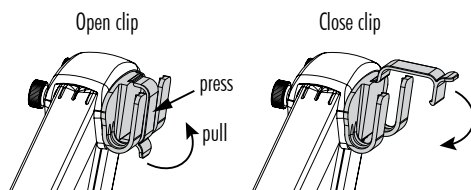

To reattach the clip onto the electrode arm:

1. Align the clip's dovetail over the slot.
2. Gently push down to slide in position.




Using the adapter

The electrode arm is ended with an electrode holder.

The holder is fitted with an adapter with three different-sized apertures:

- center-front (temperature probe only)
- center-back (adapter for pH or ORP probe)
- left and right (pH or ORP probe)

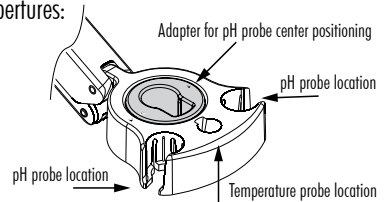

7.2. USING THE ELECTRODE HOLDER

Use the holder for electrode support and easy movement in and out of beakers and containers during calibration and sample measurement.

7.3. CONNECTING ELECTRODES & KEYBOARD

Connecting the electrodes

H11131B pH electrode attaches to the benchtop through a BNC connector, which makes attaching and removing the probe an easy process. When connected, the probe is automatically detected. With the meter off:

- Connect the probe to the BNC connection port (top right).
- Align the key and twist the plug into the socket.
- Place the probe into the holder and secure the cable. Power the unit.

Note: ORP electrodes utilize the BNC connection.


H17662-TW temperature probe attaches to the benchtop through an RCA connector. With the meter off:

- Plug the connector into the socket.
- Place the probe into the holder and secure the cable. Power the unit.

Note: Ensure connectors and plugs are correctly plugged in prior to operating the device.

- Connect a pH or an ORP half cell to the BNC connector.
- Connect a reference half-cell electrode to the socket labeled **Ref.**

A banana connector is required for a separate reference.



HI6221 Electrode compatibility

- Analog pH or ORP electrode with BNC connector (non-amplified or non-digital)
- pH or ORP half-cell sensors and separate reference electrodes with suitable jack connectors
- Hanna Instruments pH electrodes with integral temperature elements. See Accessories, Electrodes section.

Connecting a USB-A keyboard

Connect a USB's keyboard plug into the USB-A input on the back of the unit. Once connected the keyboard is automatically detected.

Users can attach a keyboard to set up calibration password, sample ID, user ID, or company/lab name.

Connecting a printer

Hanna® aims to ensure meter compatibility with USB printers but can not ensure compatibility with all models.

HI6221 can print directly to certain models of USB-dedicated printers with PCL printer language capability.

Printer components and requirements


- Printer, PCL driver compatible
- Cable
 - ▶ power cable
 - ▶ USB connector cable with two ends:
 - type B connector (plugs into printer)
 - type A connector (plugs into the USB port on the meter)


7.4. POWERING THE UNIT, SELECTING OPERATING LANGUAGE & REGIONAL PREFERENCES

1. Connect the power adapter to the rear panel of the meter.
2. Connect the power plug into the 24V power socket.
3. Press the black ON/OFF power button.

At start up, the meter briefly displays the initialization screen.



4. The instrument launches into a Tutorial.

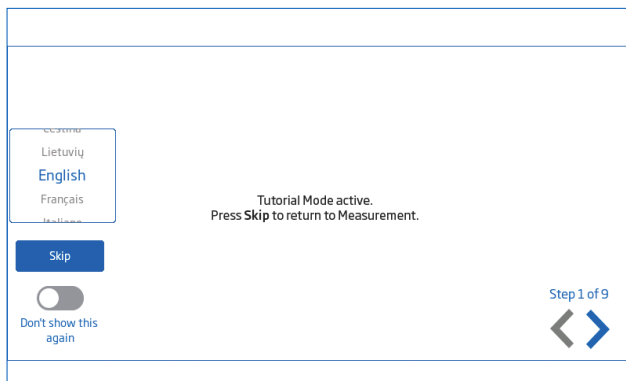Tap  to automatically enter measurement screen.



At first power on default language is English. A language window allows users to set operating language.









To configure regional preferences, from Tutorial screen:

- Tap  (direct **Menu** key) to access System Menu screen.
- Tap  (System Settings icon) and select System tab.


Users can change the date, time, and region settings, as well as language preferences.


7.5. BASIC OPERATIONS

General operating modes are setup, measurement, logging, and data sharing.






- Tap  (**Menu** key) to access:
 -  User settings
 -  System settings
 -  Measurement settings
 -  Log recall files and file management.
User can view a single sample or an interval log session, see Logging section for detailed description.
 -  Help for text and video support
- Tap  (**Home** key) to return to measurement.
- Tap  (Measurement Menu icon) to access sensor-related functions.

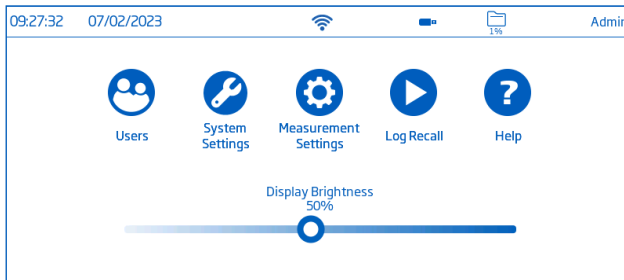8. SYSTEM MENU ITEMS

Tap  (**Menu** key) to access System Menu screen. Users must have previously logged in.



System Menu icons

Symbol	Name	Functionality
	Users	Login and rights configuration & instrument accessibility
	Settings	System configuration, connectivity and printing items
	Measurement Settings	Tap to start configuring sensor-related functions
	Log Recall	Access logged measurement data
	Help	Access video-supported outline of main instrument functionalities


Brightness control bar



Drag the slider along the control bar to adjust brightness.

8.1. USERS

Users is the first item under the System Menu and enables multiple-users configuration, rights management, and account creation.

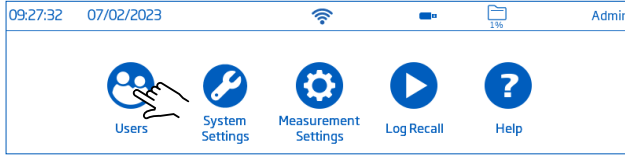


On first access, "Admin" is used as default user name and no password is required. Default options are updated from the Users menu.

Function	Administrator Rights*	Standard User
Enable account creation	✓	—
Reset password	✓	—
Delete account	✓	—
Assign administrator rights	✓	—
View/Use Factory Settings reset	✓	—
Customize settings	✓	✓
Add FTP information	✓	✓
Change password	✓	✓
View and delete log files	✓	✓


*Settings and configurations made by users with administrator rights can only be modified by users with identical rights.



Log in & Create New Account

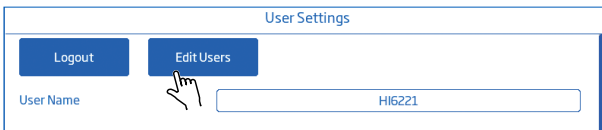
1. Power the instrument.
Wait for the initialization process to complete.
2. Tap to enter Measurement screen.
Note: Tap (under) to disable Tutorial.
3. Tap followed by .
4. Tap **Edit Users** to enter Account Management.




5. Tap to enable Account Creation and Logins. Tap to return.



6. Tap **Logout** to enter Users screen. “Admin” account is automatically created (default).
7. Tap the **plus** symbol avatar.
8. Input user name and tap .
9. Enter password and tap . Reenter password to confirm.

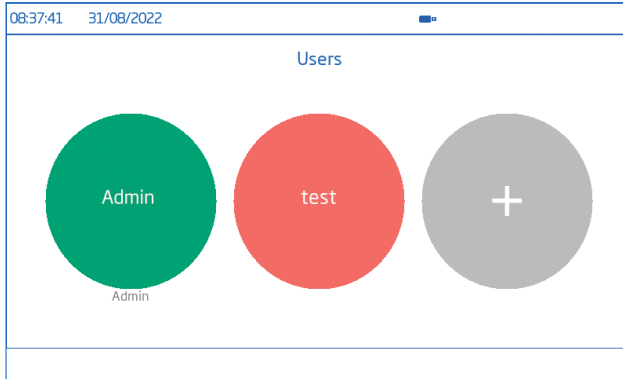


Log Out & Switch User

1. Tap  followed by **Logout**.
2. Tap on user's account avatar.
3. Input password.

Adding & Removing Users (users with administrator rights only)

1. Tap  followed by .
2. Tap **Edit Users** to enter Account Management screen and start editing.

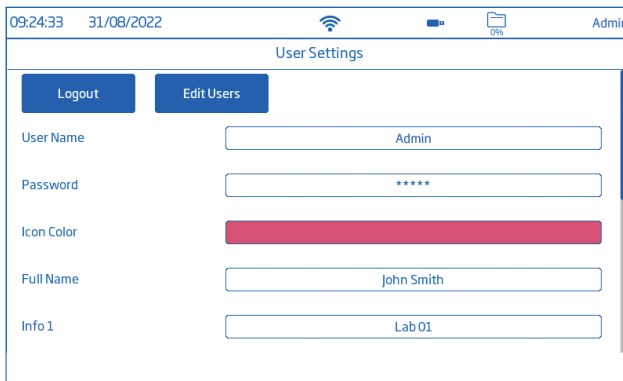

Configure user settings

Name, Password, Icon Color, Full Name, information fields, FTP-dedicated fields, Email Address


- To edit option, tap field and use the on-screen keypad to input information.
- Use the FTP dedicated fields and email address for file transfer of logged data.

Account Management


Users with administrator rights are able to:

- Enable Account Creation
 - Enable Logins
 - Enable Admin i.e. assign administrator rights to a standard user
 - Reset Password
1. Select user name from users list.
 2. Tap **Reset Password**.

The password is removed. User can set a new password.

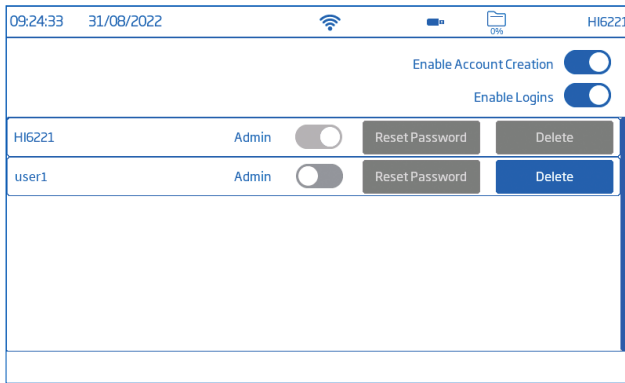

- Delete users
- Select user name and tap **Delete**. The instrument prompts for confirmation.

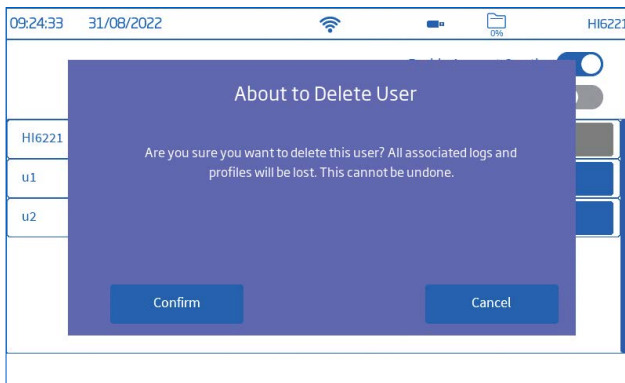


8.2. SYSTEM SETTINGS

System Settings is the second item under the System Menu.

Network, Connect & Print, System tabs permit users to navigate system settings and operations, configure network connection and architecture, connectivity and printing services, change system settings, and view meter information.

System Settings overview

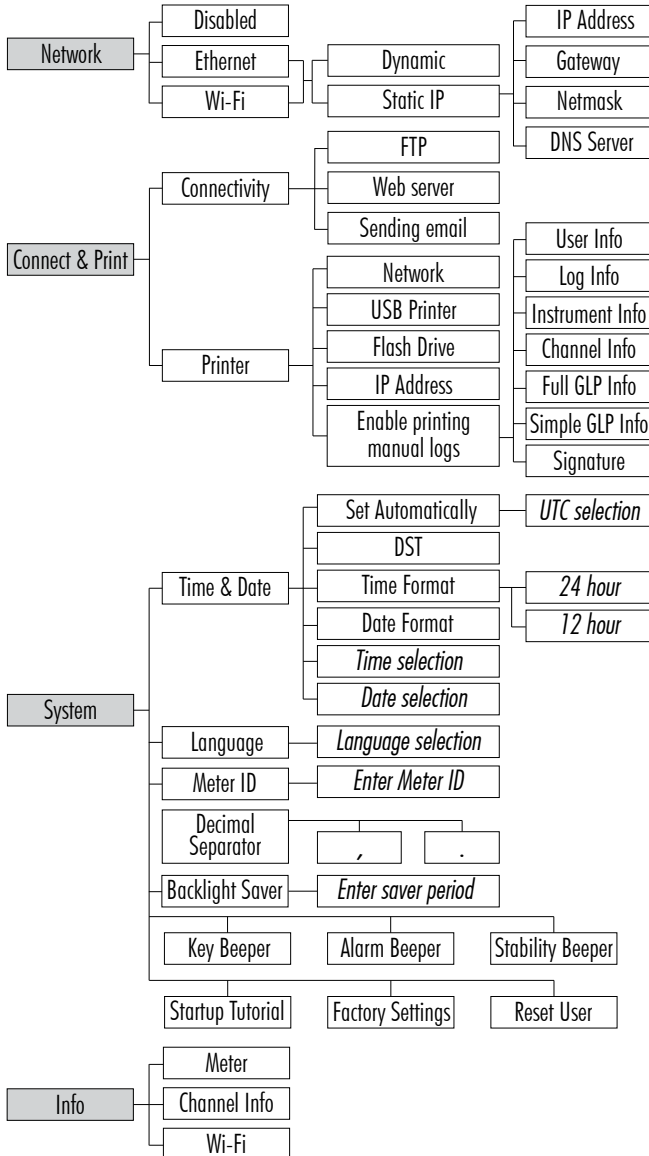


Network

Data sharing options: Ethernet, Wi-Fi, or Disabled


With connection established, IP assignment can be set as:


- Dynamic — IP Address, Gateway, Netmask, DNS Server are auto assigned
- Static — network details are filled in manually

To fill in network information:

1. Tap **IP Address** field.
2. Input address and tap .

Wi-Fi connectivity

1. Tap **Wi-Fi**.
2. Select the IP address type (Dynamic or Static).
3. Tap **Press to select network**.
4. Scan options and select preferred network.
Enter password if/when prompted.
5. Tap  to confirm.

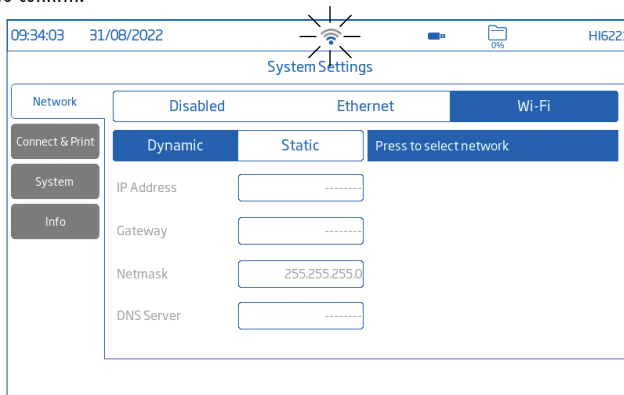

Note: With connection established, tap  or  to check IP address or verify connection status.

When attempting to connect,  icon is displayed  5 sec. .


Connect & Print

Options: Connectivity, Printer

Tap  to enable (disable) following **connectivity** options:

- FTP access to meter: log file transfer to an FTP site and meter FTP server connection to client (log download)
- Meter web server: log file download to a web client
- Sending emails: log file transfer via email

Note: Email address is entered under User.

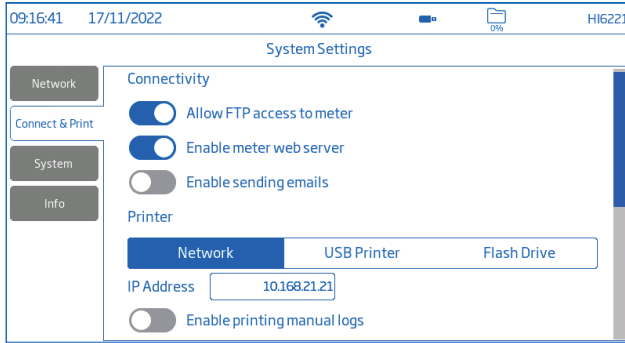


Printer

Options: Network, USB Printer, Flash Drive

- Select **Network** to connect a printer in the same network. Tap to enter IP address.
- Select **USB Printer** to connect a printer via USB-A port.
- Select **Flash Drive** to export log files directly to USB Flash Drive.
- Tap **Enable printing manual logs** to send files to configured printer. Tap to enable for printing: User, Log, Instrument, and Channel information, Full GLP, Simple GLP, Signature.

Note: Printer options are available with a printer connected only.

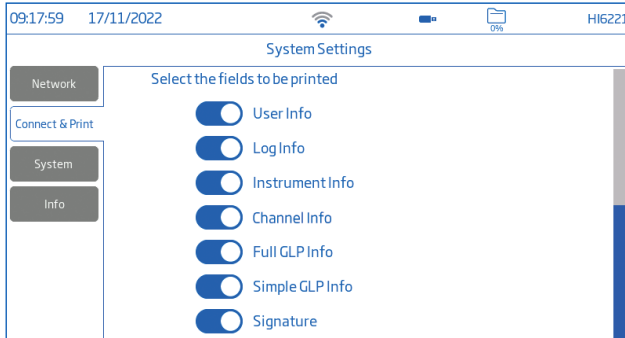

System



Options: Time, Date, Language, Meter ID, Decimal Separator, Backlight Saver, Beepers, Startup Tutorial, Factory Settings, Reset User

Note: Use the scroll bar to view or select from entire settings list.

Time & Date

Tap to enable (or disable):

- **Set Automatically** (meter must be connected to the internet)
 - ▶ Direct selection from scrollable list of options
 - ▶ UTC options:
 - from UTC 00:00 to UTC + 14:00
 - from UTC 00:00 to UTC - 12:00 (half hour increments)
- **DST** (Daylight Savings Time) seasonal time change is used in some locations that advances clocks (typically by one hour) during warmer months.

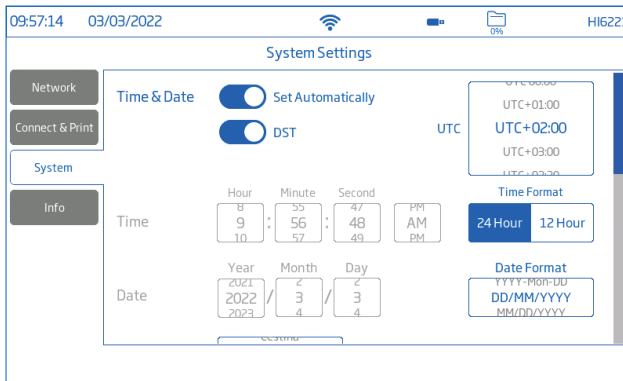

Time: Hour, Minute, Second, time of day (AM or PM), time format (24 or 12 Hour)

Note: Set Automatically must be disabled

Date: Year, Month, Day, choice of display formats (DD-Mon-YYYY; YYYY-Mon-DD; DD/MM/YYYY; MM/DD/YYYY; YYY/MM/DD; YYYY-MM-DD; Mon DD, YYYY)


Note: Set Automatically must be disabled

Language: select from list of supported options to change meter's interface language

Meter ID


Name the meter with a discrete name, location, or number.

Tap  to save.

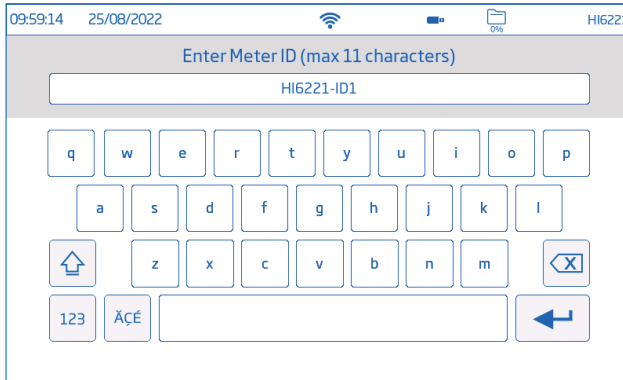

Tap  or corresponding tab to enable (or disable) following settings:


- **Decimal Separator:** comma or period
- **Backlight Saver:** enabled, 1 to 60 minutes (or disabled)
If the backlight turns off after the set period of time, tap to turn it back on.
- **Beeper:** Key, Alarm, Stability
When enabled, an audible signal alerts users in the event of a wrong key press, an alarm condition, or the stability threshold being exceeded.
- **Startup Tutorial:** if disabled, the meter does not launch into Tutorial at power on.

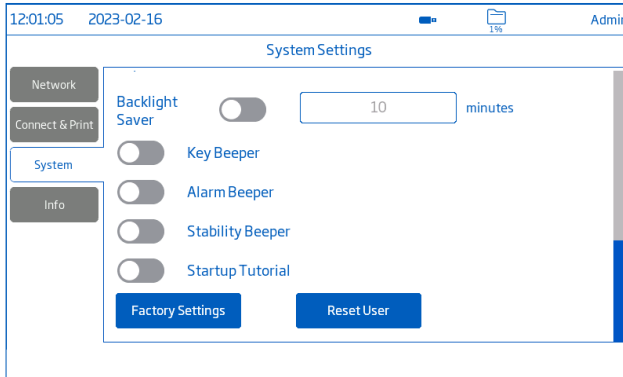

Factory Settings

Option restores system settings i.e. resolution for measured data, temperature unit, view mode, and alarm to original factory values. Restoring factory settings deletes all user information, logs, or configured measurement profiles. When option invoked, the instrument asks for confirmation.

Note: Option available to users with administrator rights only.

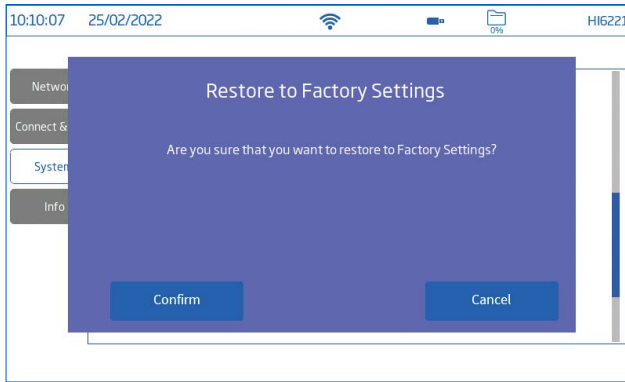


Reset User

Option restores default settings for this user. All data (including profiles and log files) specific to this user will be permanently deleted, except for the username and password.

When option invoked, the instrument asks for confirmation.


Info

Read-only item displays information on meter, channel serial number, and Wi-Fi firmware version.

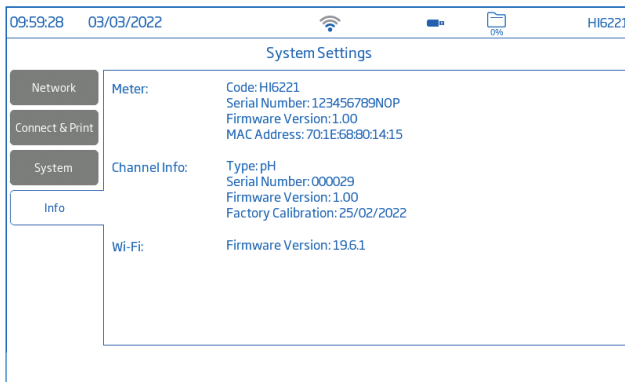

8.3. MEASUREMENT SETTINGS

Measurement Settings is the third item under the System Menu and allows setting calibration, reading, temperature, view, alarms, logging and measurement profile options.

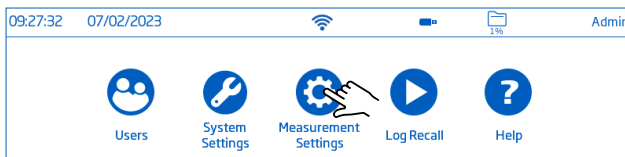

Measurement Settings Overview

Calibration, Reading, Temperature, View, Alarms, Logging, Profile tabs help user navigate through all measurement operations. The following table presents an overview of possible functions.

Calibration

	pH	mV	Rel.mV
Last Calibration	Calibrate Clear	✓	Calibrate Clear
Buffer Entry Type	Automatic Semiautomatic Manual	✓	✓
Buffer Auto Confirmation	Enabled Disabled	–	–
First Calibration Point	Point Offset	✓	✓
Calibration Reminder	Disabled Daily Periodic	✓	Disabled Daily Periodic
Buffer Group	User defined	✓	✓

Reading

	pH	mV	Rel.mV
Resolution	0.1 0.01 0.001	1 0.1	1 0.1
Stability Criteria	Accurate, Medium, Fast		
Reading Mode	Direct, Direct/Autohold		

Temperature

	pH	mV	Rel.mV
Temperature Source	Automatic, Manual		
Temperature Unit	°C, °F, K		
Manual	–20.0 to 120.0 °C –4.0 to 248.0 °F 253.2 to 393.2 K		
Isopotential Point	user defined (–2.000 to 20.000)	✓	✓
User Temperature Calibration	Calibrate, Clear		

View

		pH	mV	Rel.mV
View Type		Basic Simple GLP Full GLP Graph Table	Basic Graph Table	Basic Simple GLP Graph Table

Alarms

		pH	mV	Rel.mV
High / Low pH		-2.000 to 20.000	✓	✓
High / Low mV		✓	-2000.0 to 2000.0	
High / Low Temperature		-20.0 to 120.0 °C -4.0 to 248.0 °F 253.2 to 393.2 K		

Logging


		pH	mV	Rel.mV
Logging Type		Automatic Manual Autohold (Direct/Autohold Reading mode only)		
Sampling Period (Automatic type only)		1, 2, 5, 10, 30 sec. 1, 2, 5, 10, 15, 30, 60, 120, 150, 180 min.		
File Name (Manual & Autohold only)		Create Unnamed Log		
Log Note		User defined		
Log Info 1 through to 4		User defined		
Sample ID Prefix (Manual or Autohold only)		0 to 999		

Profiles

		pH	mV	Rel.mV
Profile Feature		Enable Disable		
Current Profile		Save As Save Delete		
Load Profile		Previously defined profiles		

8.4. LOG RECALL

Log Recall is the fourth item under the System's Menu and allows data selection, viewing, sharing, and deletion. Logged data is retrieved by the user that has logged the measurement.

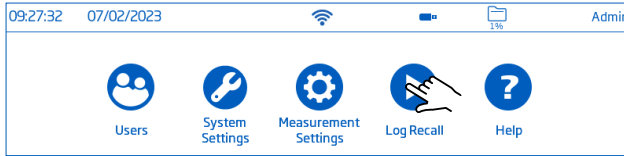

- Data is stored in parameter-specific .CSV files: pH, mV, and Rel.mV.
- Storage location is independent and organized in lots.
- A lot (file) can store 1 to 50 000 log records i.e. saved measurement data points.
- One user can store a minimum of 1 000 000 data points.

View

Data can be viewed, plotted (graph), or tabulated (complete with date, time, notes).

From the System Menu screen:

1. Tap (Log Recall). The instrument displays the Log Recall screen.
Tap on corresponding table header element to set the log information ordered by Name, Parameter, Start/Stop time stamp, #Samples.
Tap the up arrow to reverse order.
2. Tap to select .CSV file.
3. Tap **View**.

Note: Option available with .CSV file selected only.

The screenshot shows the 'Log Recall' screen with a table of logged data. The status bar at the top shows '10:04:39', '03/03/2022', signal strength, Wi-Fi, battery, and 'HI6221' user. The table has columns for Name, Parameter, Start/Stop, and #Samples. The table is sorted by Start/Stop time.


Name	Parameter	Start/Stop	#Samples
20220326_085354-pH_auto.csv	pH	08:53:54 26/03/2022 08:53:57 26/03/2022	4
20220326_085358-pH_auto.csv	pH	08:53:58 26/03/2022 08:54:06 26/03/2022	9
20220326_114046-pH_auto.csv	pH	14:39:57 26/03/2022 14:40:15 26/03/2022	19
20220326_114309-pH_man-Lab12_002.csv	pH	14:40:47 26/03/2022 14:41:04 26/03/2022	18
20220326_114523-pH_man-Lab12_003.csv	pH	14:44:35 26/03/2022 14:44:36 26/03/2022	27
20220326_115959-mV_man-Lab12_004.csv	mV	14:46:01 26/03/2022 14:46:02 26/03/2022	19

4. Tap  or  icon to have logged data displayed in tabulated form or plotted.

10:06:02 03/03/2022 HI6221

20220326_114523-pH_man-Lab12_003.csv

Index	Date	Time	pH	pH-mV	T[°C] ATC	Notes
1	26/03/2022	14:45:23	9.0	-116.7	25.0	"H"
2	26/03/2022	14:45:24	9.0	-116.7	25.0	"H"
3	26/03/2022	14:45:25	9.0	-116.7	25.0	"H"
4	26/03/2022	14:45:26	9.0	-116.7	25.0	"H"
5	26/03/2022	14:45:28	9.0	-117.1	25.0	OK
6	26/03/2022	14:45:29	8.8	-108.0	25.0	OK
7	26/03/2022	14:45:30	8.8	-108.2	25.0	OK
8	26/03/2022	14:45:31	8.8	-108.2	25.0	OK
9	26/03/2022	14:45:32	8.7	-99.4	25.0	OK
10	26/03/2022	14:45:33	8.7	-99.5	25.0	OK

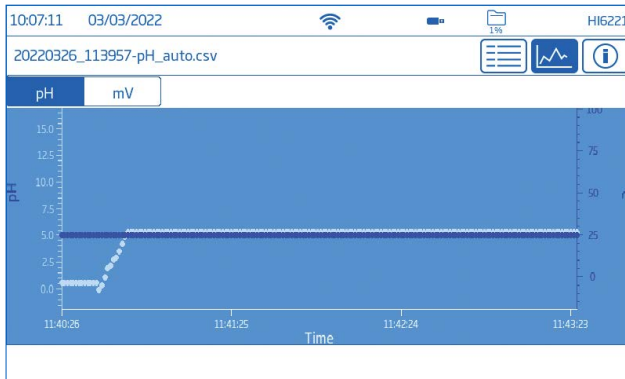

5. Tap  icon and scroll through USER, LOG, INSTRUMENT, CHANNEL, GLP DATA information.

10:07:53 03/03/2022 HI6221


20220326_113957-pH_auto.csv

USER INFO
 User Name: HI6221
 Full Name: John Smith
 Info 1: Hanna Instruments
 Info 2: Addr
 Info 3:
 Info 4:


LOG INFO
 Log Note:
 Log Info 1:
 Log Info 2:


Select (Deselect) All

To export to a USB-A flash drive:

1. Tap  (Log Recall) to access the log history.
2. Tap **Select All** button to select entire log history.
With all files selected, tap **Delete** to empty the log or tap **Share** to transfer data.
3. Tap **Deselect All** to clear selection.

Delete

1. Tap  (Log Recall) to access the log history.
2. Tap to select required .CSV file (one file) or tap **Select All**.
3. Tap **Delete**.
4. The instrument prompts for confirmation.
Deleted files can not be recovered and Log Recall screen is displayed blank.

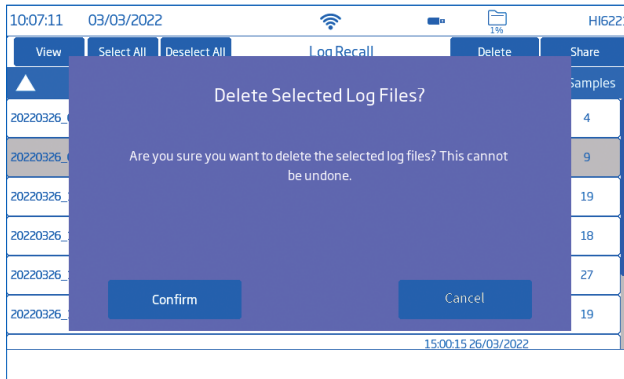



Share

Options: USB-A, FTP, Email, Print, Web server

USB-A and USB-C

Plug the USB flash drive into the USB port located on the back.

1. Tap  (Log Recall) to access the log history.
2. Select file (files) for transfer or use **Select All** option.
3. Tap **Share**. Pop-up flyout is displayed.
4. Tap to select USB-A or USB-C.
 is displayed for transfer in progress.
5. Transfer completion is confirmed and the instrument returns to Log Recall screen.

FTP

HI6221 can act as an FTP server (host) or client. Meter has to be connected to the internet and **Allow FTP access to meter** enabled.

- Use meter's IP address and password to connected and view logged files.
- Enter in the FTP dedicated fields own server information to export logged files to the FTP server.
- Configure FTP server info in the User menu (😊) to use the meter as an FTP client and upload files to an FTP server.

Connect via **FTP to meter server**:

1. On preferred FTP software, type the meter's IP address in the dedicated Host field.
2. Enter the username and password of the user currently logged in.
3. Connect to view the files logged on the meter.



Connect the **meter to an FTP server** and share logs:

1. In Users menu, type selected server's IP address, username, and password.
2. From System Menu, tap 🎮 . Log Recall screen opens up.
3. Select file (files) for transfer.
4. Tap **Share**. Pop-up flyout is displayed.
5. Tap to select FTP. The files are being transferred in the root folder of the server.

FTP server installation and configuration

- PC running Windows10 or later
- Password protected Windows account
- FTP server must be allowed through the Windows Firewall

Installation

1. Navigate to **Start > Control Panel > Administrative tools > Server Manager**.
2. Go to **Roles** and expand **Web Server**.
3. Right click on **Web Server** and then click on **Add Role Services**.
4. Go to **Role Services** and check **FTP Server**.
5. Ensure **IIS Manager** (Internet Information Services) is checked under **Management Tools**.
6. Click **Next** followed by **Install**.
7. Wait for installation to complete.

Configuration (PC must be running Windows10 or later)

1. Navigate to **Start > Control Panel > Administrative tools > IIS Manager** (Internet Information Services).
2. Double click to expand the **IIS Manager** console.
3. Right click on **Sites**, on the Connection pane.
4. Click on **Add FTP Site**, to select. Type the FTP server name and the path to be used for file transfer


Note: Select *Make New Folder* to create a designated folder to store FTP files.

5. Click **Next**.
6. In the Binding and SSL Settings window keep all default settings but change the SSL option to **No SSL**.
7. Click **Next**.
8. When prompted to authenticate and authorize information, select **Basic and Specified** users.
9. Type local account name to gain access to the server.
10. Check both **Read** and **Write** options.
11. Click **Finish**.

Email

Meter has to be connected to the internet and **Enable sending emails** enabled (see System Settings, Connect & Print section).

Tap  to access the Users menu and input email address.

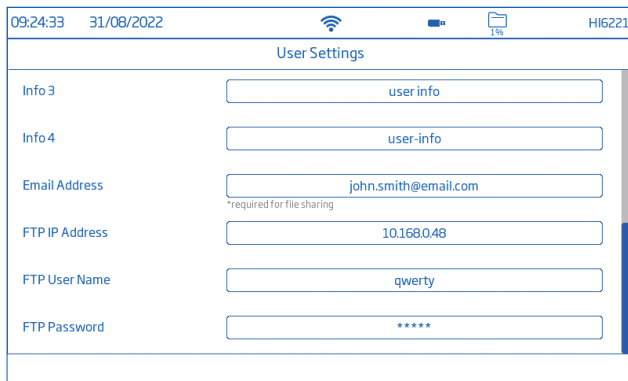

09:24:33 31/08/2022 HI6221

User Settings

Info 3 user info


Info 4 user-info

Email Address john.smith@email.com
*required for file sharing

FTP IP Address 10.168.0.48

FTP User Name qwerty

FTP Password *****

1. From System Menu, tap  to access Log Recall.
2. Select file(s) for transfer or use **Select All** option.
3. Tap **Share**. Pop-up fly-out is displayed.
4. Select **Email**.
5. Transfer completion is confirmed and the instrument returns to Log Recall screen.



10:12:58 03/03/2022 HI6221

View Select All Deselect All Log Recall Delete Share

Name	Parameter	Start/Stop	Files
20220326_113957-pH_auto.csv	pH	14:39:57 26/03/2022 14:40:15 26/03/2022	
20220326_114046-pH_auto.csv	pH	14:40:47 26/03/2022 14:41:04 26/03/2022	
20220326_114309-pH_man-Lab12_002.csv	pH	14:44:35 26/03/2022 14:44:36 26/03/2022	
20220326_114523-pH_man-Lab12_003.csv	pH	14:46:01 26/03/2022 14:46:02 26/03/2022	
20220326_115959-mV_man-Lab12_004.csv	mV	15:00:15 26/03/2022 15:00:16 26/03/2022	11
20220326_120059-relmV_auto.csv	Rel. mV	15:01:00 26/03/2022 15:01:42 26/03/2022	43

Share To:
USB-A
FTP
Email
Print
Cancel

Print

- Connect either a printer (Network or USB) or plug-in a USB Flash Drive (see System Settings, Connect & Print section).
- Tap **Print** and follow on-screen instructions.

Web server


Any browser can be used to access the web server and download log files. Meter has to be connected to the internet and **Enable meter web server** enabled (see System Settings, Connect & Print section).

Note: Both the meter and the device the browser is accessed from have to be connected at the same network.

1. Tap  for IP address and type address in the browser.



2. Enter the username and password of current user to gain access to logs and tags. Click on file to download to the PC.

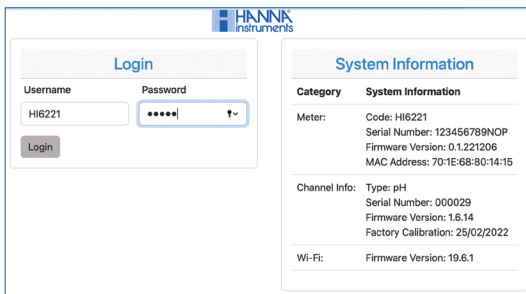

logs

File Name	Parameter	Number of Entries	Start Time	Stop Time		
20221117_084933-pH_auto.csv	pH	36	08:49:33 17/11/2022	08:50:08 17/11/2022	Download	View
20221117_085027-pH_auto.csv	pH	42	08:50:27 17/11/2022	08:51:08 17/11/2022	Download	View
20221117_085116-pH_auto.csv	pH	26	08:51:17 17/11/2022	08:51:42 17/11/2022	Download	View
20221117_085705-pH_auto.csv	pH	2	08:57:05 17/11/2022	08:57:06 17/11/2022	Download	View
20221117_090941-pH_new_log_002.csv	pH	13	09:09:41 17/11/2022	09:10:10 17/11/2022	Download	View
20221208_082926-mV_auto.csv	mV	26	08:29:26 08/12/2022	08:29:51 08/12/2022	Download	View

PC Connection

The logged data can be transferred from the meter to a PC.


- Use the USB-C cable to connect the meter to the PC.
- The meter will appear as a flash drive on the computer.
- Save files to the PC. All logs will be listed as .CSV files.


The .CSV files may be opened with any text editor or spreadsheet application.


All features of the spreadsheet program can be used to analyze and graph the data.

8.5. HELP

Help is the fifth item under the System Menu.


- Tap  to access support and navigate through an overview of system's main functionalities.

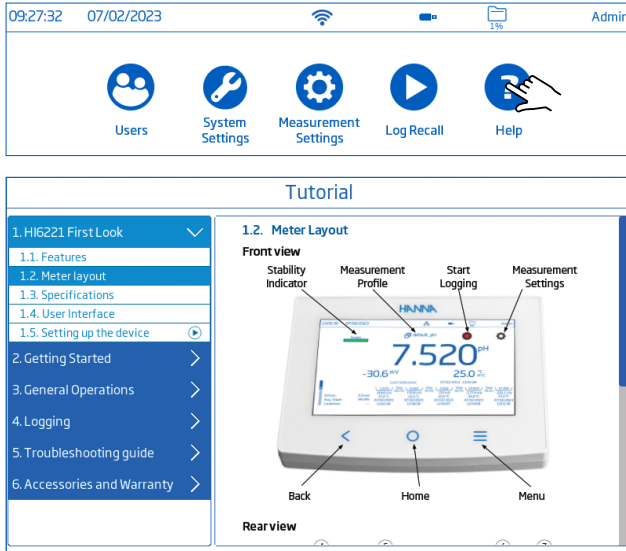

- Tap to play (stop) video-supported segments:
 - ▶ 1.5. Setting up the device
 - ▶ 3.1. Calibration
 - ▶ 3.2. Reading measurements
- Tap  once to increase video speed.
 - ▶ The meter supports, with each tap, three playback speeds: normal (x1), medium (x2), and fast (x4).

9. MEASUREMENT & ELECTRODE SETUP MENU

From the Measurement screen, tap  to access system and measurement configuration tabs. Alternatively, tap  (Menu key) then tap .

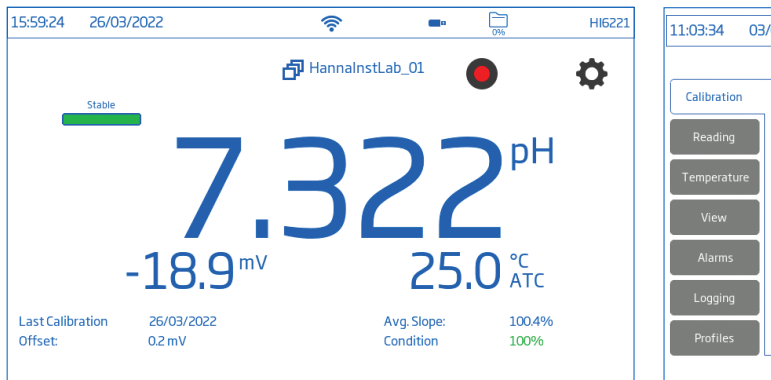

9.1. CALIBRATION

Options: Last Calibration, Buffer Entry Type, Buffer Auto Confirmation, First Calibration Point, Calibration Reminder, Buffer Group

Last Calibration: calibrate or clear a previous calibration

Buffer Entry Type

- **Automatic:** meter selects the closest buffer value to that of the pH sample being measured
- **Semiautomatic:** meter selects the closest buffers to that of the pH sample being measured. The user has the option to manually select between buffers that are close in value.
- **Manual:** user manually selects the required buffer value

Buffer Auto Confirmation: recognized buffer value automatically accepted pending stable reading


First Calibration Point

- **Point:** a new buffer value can be added to an existing calibration. This prompts an automatic reevaluation of the electrode slope.
- **Offset:** the new buffer calibration point can create a constant offset to all existing pH calibration data performed with a minimum of two pH buffers.

Calibration Reminder


- **Daily-**calibration interval (hours and minutes)
- **Periodic-**calibration interval (days, hours, minutes)

“Calibrate probe” message runs along the bottom of the measurement screen if calibration is not done within set interval.

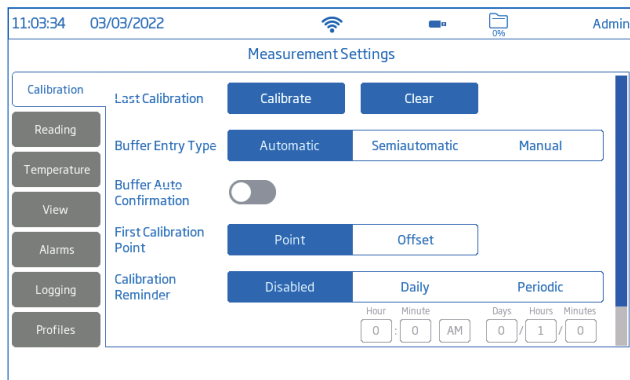


Buffer Group

Option used for Automatic calibration.

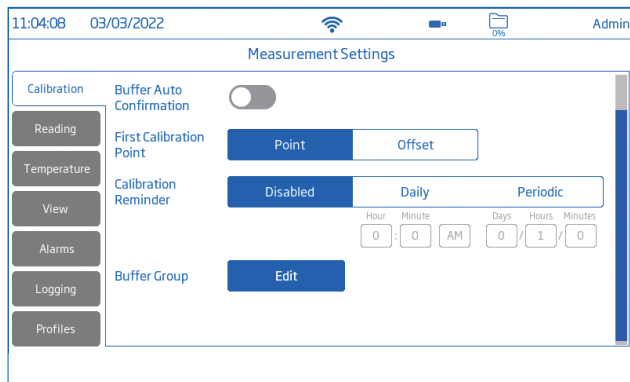

To move from **Available Standard/Custom Buffers** to the **Buffers in Use** column (up to five buffers), select buffer and forward arrow.


To edit and add a custom buffer, from the Measurement screen:

1. Tap .
2. Tap **Reading** tab and set pH Parameter.
3. Tap **Calibration** tab.
4. Tap **Edit** next to Buffer Group.
5. Select from available input field in the Available Custom Buffers list.
6. Tap **Edit** to enter buffer value at the calibration temperature value and **Enter** to confirm.
7. Repeat with up to 5 custom values.

Once the maximum number has been reached, to add another custom value, delete a previously set value.

9.2. READING

Options: Parameter, Resolution, Stability Criteria, Reading Mode

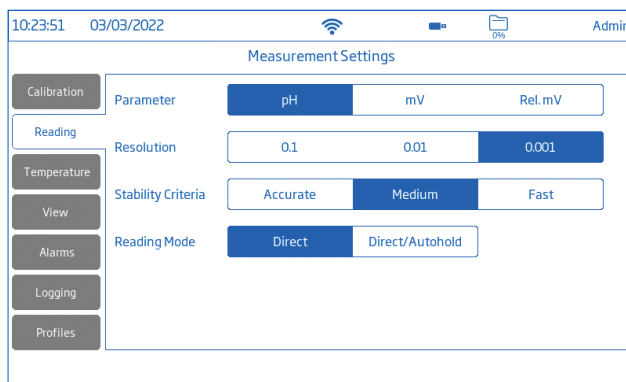

Parameter

Options: pH, mV, Rel. mV



Tap to select desired measurement configuration: pH, mV (ORP), Rel. mV (ORP with calibration).

Resolution

Tap to select measurement resolution based on selected parameter.

Stability Criteria






Set the stability criterion for selected mode based upon selected stability setting.

While the measurement is changing, the stability indicator is shown partially (); when the criteria is reached the indicator is displayed as a full green bar ().


- **Accurate:** for applications where high accuracy is required
Measurement is recognized as stable using more critical criteria evaluating measurement fluctuations.
- **Medium:** for applications where average accuracy is accepted
Measurement is recognized as stable using less critical criteria evaluating measurement fluctuations.
The measurement may still change after registering stable.
- **Fast:** for applications where speed of delivery has priority

Reading Mode

Options: Direct, Direct/Autohold

- **Direct:** as measurement changes measurement stability is continuously evaluated. Unstable (blinking) or stable indicator are displayed above the progress bar.
- **Direct/Autohold:**  (lock icon) is displayed between the log and Measurement Menu icons.
 - ▶ Tap  to initiate a measurement.
 - ▶  or  is displayed depending on selected parameter.
 - ▶  is displayed blinking until the measurement is stable.

- ▶ When stable, the indicator stops blinking and measurement freezes at current value.
- ▶ Tap **pH** or **mV** to return to direct measurement.

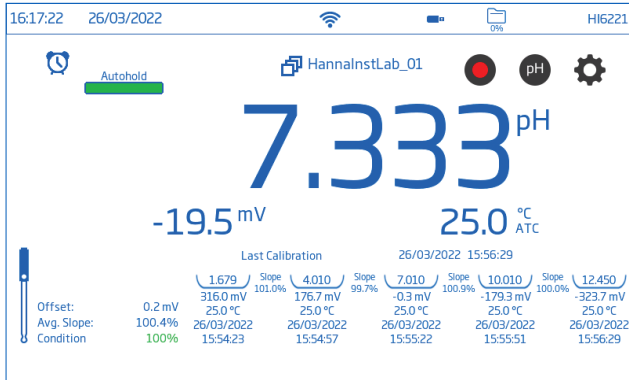

9.3. TEMPERATURE

Options: Temperature Source, Temperature Unit, Manual, Isopotential Point (pH parameter only), User Temperature Calibration

15:39:23 26/03/2022 Admin

Measurement Settings

Calibration

Reading

Temperature

View

Alarms

Logging

Profiles

Temperature Source: Automatic Manual

Temperature Unit: °C °F K

Manual: °C

Isopotential Point: pH

User Temperature Calibration: Last Calibration: 26/03/2022

Temperature Source: Automatic, Manual

User can select between physical temperature input source (Automatic) and entering sample temperature value manually (Manual).

- **Automatic** (with temperature probe): ATC is displayed next to the temperature measurement on the pH display. The mV/Rel. mV display indicates temperature value.
- **Manual** (without temperature probe): MTC is displayed next to the temperature measurement on the pH display. Manual is displayed next to the temperature measurement on the mV/Rel. mV display. Sample's temperature needs to be entered.

Temperature Unit: Celsius, Fahrenheit, Kelvin degrees

- Tap to select unit.

Manual

To manually input value (**Manual** selected under Temperature Source or no temperature probe):

1. Select temperature unit.
2. Tap on Manual Temperature field. Use the on-screen keypad to enter sample's temperature.

Isopotential Point: —2.000 pH to 20.000 pH

Isopotential point is the point at which temperature has no effect on pH readings. Unless noted with electrode, use 7.000 pH.

- Tap on the field and use the on-screen keypad to input value (pH measurement only).

User Temperature Calibration: Calibrate or Clear

To perform a new calibration:

1. Tap **Calibrate**.
2. Place the probe and a reference thermometer (with 0.1 resolution) into a stirred container of water. Allow for the reading to stabilize.
3. If the displayed value is different than the reference thermometer reading, tap **Preset Temperature** and use the on-screen keypad to enter the value.
4. Tap **Save** to confirm and save data.

15:37:16 26/03/2022 HI6221

Calibrate temperature

Measured Temperature: °C

Preset Temperature: °C

Check if the displayed value is different than the reference thermometer reading.
If yes, touch the preset temperature value to change it, else press 'Save' to save the calibration data.

Clear Calibration Cancel Save


9.4. VIEW

pH: Basic, Simple GLP, Full GLP, Graph, Table

mV: Basic, Graph, Table


Rel.mV: Basic, Simple GLP, Graph, Table

- Select preferred display configuration from View Type window.

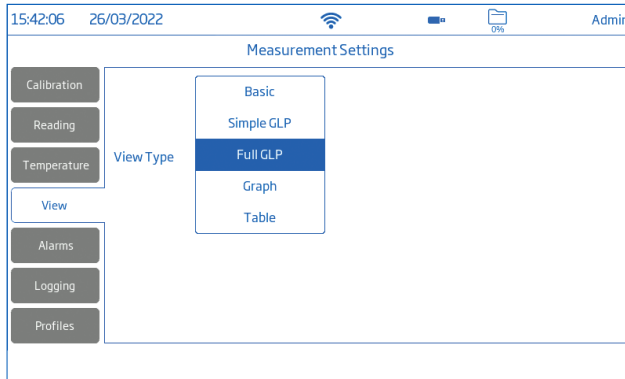


Basic

Screen displays the measured value, measurement unit as well as temperature-probe status.

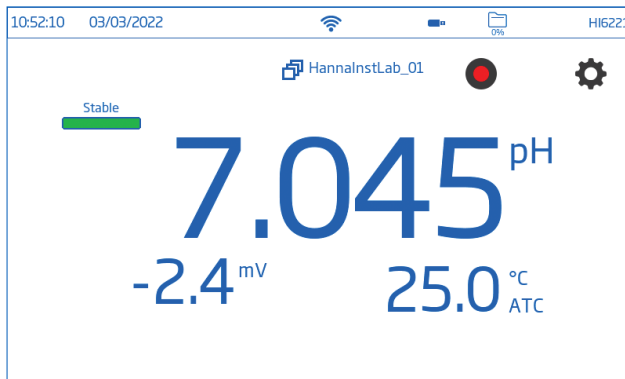

Simple GLP


In addition to data displayed when Basic option is selected, screen displays: last calibration date and time, Offset value, average slope (Avg.Slope), and electrode condition (Condition).

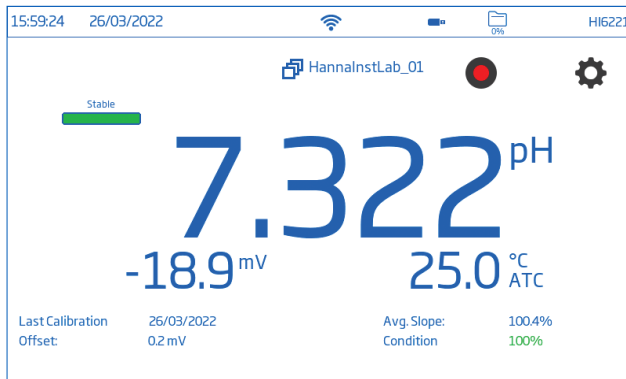

Note: If no calibration has been made, Not Calibrated is displayed.

Full GLP

In addition to data displayed when Simple GLP option is selected, screen displays: electrode symbol, used buffers as well as calibration date, time, and temperature probe status.

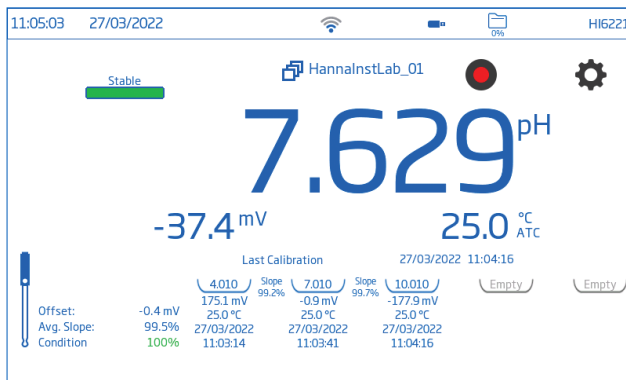


Graph

When Graph is selected, the measured value is plotted as a graph.

To zoom in on a graph:

1. Select Time or parameter axis.
2. With axis selected, pinch or drag on the display.

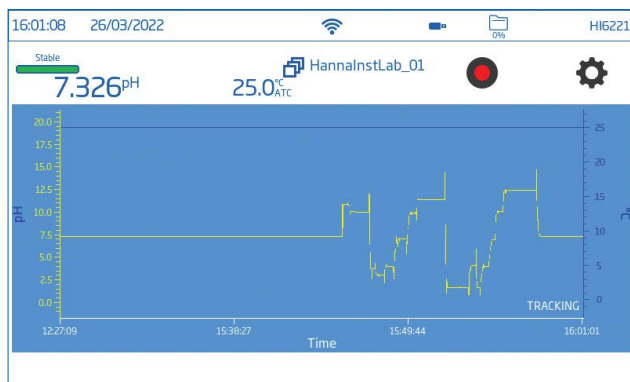

Table

When Table is selected, the measured values are displayed tabulated (complete with date, time, and notes made during logging). The newest data is displayed on the top of the table.

pH	mV	T(°C)	Time	Date	Notes
7.521	-30.6	25.0	13:07:56	07/02/2023	
7.521	-30.6	25.0	13:07:55	07/02/2023	
7.521	-30.7	25.0	13:07:54	07/02/2023	
7.521	-30.7	25.0	13:07:53	07/02/2023	
7.521	-30.7	25.0	13:07:52	07/02/2023	
7.521	-30.6	25.0	13:07:51	07/02/2023	
7.521	-30.7	25.0	13:07:50	07/02/2023	
7.521	-30.7	25.0	13:07:49	07/02/2023	
7.521	-30.6	25.0	13:07:48	07/02/2023	
7.521	-30.7	25.0	13:07:47	07/02/2023	
7.520	-30.6	25.0	13:07:46	07/02/2023	

9.5. ALARMS

Options

pH: High or Low pH, High or Low Temperature


mV & Rel.mV: High or Low mV, High or Low Temperature


Users can set the threshold limits for the measured parameters. When the measurement exceeds the high-threshold value or drops below the low-threshold value, the alarm is triggered and an alarm message is displayed on the message banner.

If the Alarm Beeper is enabled (See: System Menu Items / System Settings / Alarm Beeper), an audible beep will be heard.

Note: High-parameter values cannot be lower than low-parameter ones.

To set an alarm limit:

1. Tap  to enable low or high threshold option.
2. Use the on-screen keypad to enter the value.
3. Tap **Enter** to confirm or **Cancel** to exit and return to measurement setting options.

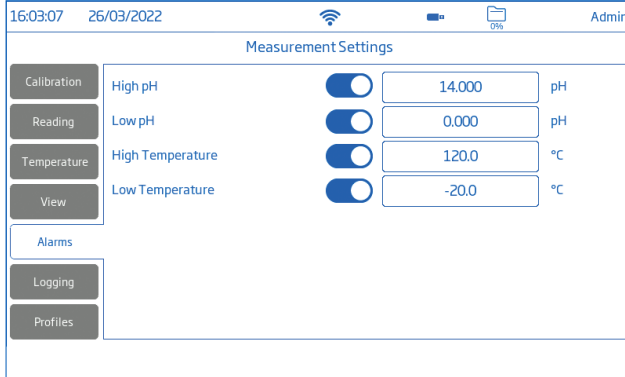


 (alarm icon) is displayed on the measurement screen when an alarm is active.



9.6. LOGGING

Options: Logging Type, Sampling Period, File Name, Log Note, Log Info, Sample ID

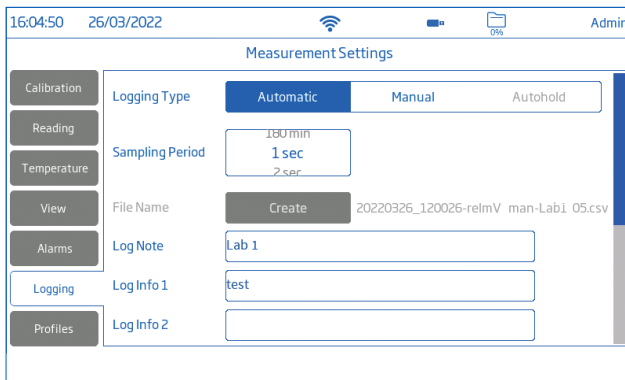

16:06:20 26/03/2022 Admin

Measurement Settings

Calibration Log Note

Reading Log Info 1

Temperature Log Info 2

View Log Info 3

Alarms Log Info 4

Logging Sample ID None Increment Manual

Profiles

Sample ID Prefix 0 9 9 0
1 1 0 0
2 1 1 1


Logging Type

- **Automatic**

Data is logged automatically at predefined time intervals (i.e. Sampling Period). A file name is automatically generated, complete with year/month/day, and logging time. Files are identified by parameter e.g.:

- pH log files: 20220329_085101-pH_auto.CSV
- mV log files: 20220429_084105-mV_auto.CSV
- Rel.mV log files: 20220309_095704-relmV_auto.CSV

- **Manual**

Measured data is logged every time  is tapped.

- **Autohold**

Available with Direct/Autohold reading mode only.

Note: Manual and Autohold records are stored in the same log file, i.e. data logged on different days is stored in the same lot. Automatic records are stored separately.

Data logged with Autohold option selected, is identified by "H" in the Notes column.

Sampling Period

Option available with Automatic logging type selected only.

Time-interval options are selected from scrollable list.

File Name

Available with **Manual** and **Autohold** logging type selected only.

To create a file name, from Logging screen:

1. Tap **Create**.
2. Use the keypad and enter file name (maximum 13 characters).
3. Tap **Enter** to confirm.


Log Note & Log Info

Notes on measured data are saved together with logged data.

Sample ID

Manual and autohold samples can be labeled with a numerical ID (increments with each new sample logged), a text label, or a text label with numerical ID.


With **Increment** selected:

1. Tap **Sample ID Prefix**.
2. Use the on-screen keypad to enter a text prefix, of maximum 15 characters, to the sample name.
3. Tap .
4. Select ID number from scrollable list.

9.7. PROFILES

Options: Profile Feature, Current Profile (configure), Load Profile (previously configured)

Profile Feature option can be enabled or disabled.

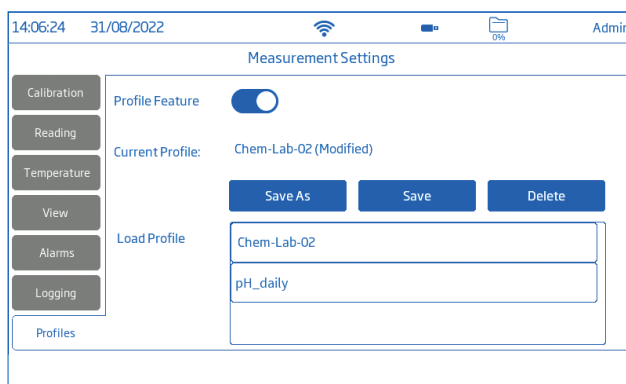



Current Profile

A profile is a sensor setup complete with required measurement unit, temperature unit, display preference, and alarm threshold options.

Once saved the profile can be loaded for applications that require similar configurations.

To save a profile, having previously configured all other application-specific options, from the Measurement screen:

1. Tap .
2. Tap **Profiles** tab.
3. Tap **Save As** and use the keypad to enter profile name.
4. Tap  to confirm.

Once saved, profile name is added to the Load Profile list.

Load Profile

To select from list of predefined profiles:

1. Tap to select from the **Load Profile** list.
2. Profile name is automatically entered in the **Current Profile** field.
3. Start measuring.

10. CALIBRATION PROCEDURE

Calibration Overview (compiled UI symbols)

Automatic Semiautomatic Manual

Stable 12.426 pH -320.5 mV ATC 25.0°C

Calibrate pH

Confirm Buffer... Touch Confirm Buffer to update the calibration and move to the next buffer.

Clear Calibration Cancel Save Confirm Buffer

Current MOD1 pH calibration status		
4.010	Slope 99.2%	7.010 Slope 99.7%
175.1 mV	-0.9 mV	177.9 mV
25.0 °C	25.0 °C	25.0 °C
27/03/2022 11:03:14	27/03/2022 11:03:41	27/03/2022 11:04:16

Last Calibration 27/03/2022 11:04:16

4.010	Slope 99.2%	7.010	Slope 99.7%	10.010	Empty	Empty
175.1 mV	-0.9 mV	-0.9 mV	-177.9 mV			
25.0 °C	25.0 °C	25.0 °C	25.0 °C			
27/03/2022 11:03:14	27/03/2022 11:03:41	27/03/2022 11:03:41	27/03/2022 11:04:16			

Offset: -0.4 mV
Avg. Slope: 99.5%
Condition: 100%

1 Calibration type

2 Forward or backward navigation, sequence of steps

3 Save and Confirm buffers, calibration procedure

4 Standard Buffers trays, with buffer selected for transfer (rectangular outline)

5 Custom Buffers trays

6 Buffer management

7 Buffers in use

8 Buffer symbol: **S** (standard) or **C** (custom)

9 Electrode calibration details for used buffer

10 Electrode symbol with Offset, Average Slope, and electrode condition (indication of electrode status)

10.1. pH CALIBRATION

Calibration Guidelines

- Set up a routine service schedule where measurement integrity is validated.
- Do not handle the sensing surfaces of the sensors.
- Avoid rough handling and abrasive environments that can scratch the reactive surfaces of the sensors.
- For best technique, use a rinse beaker and a separate calibration beaker for each buffer.
Discard buffers after use.
- Do not return the used buffers to the bottles of “fresh” buffer.
- For measurements across a temperature gradient (when water temperature is drastically different from the buffers), allow the electrodes to reach thermal equilibrium before conducting calibrations or making measurements.
- During calibration the temperature probe should be in the calibration buffer.

pH Calibration Type

Automatic: instrument automatically selects closest buffer to the pH value being measured from all active buffers selected as Buffers in Use

Semiautomatic: instrument automatically selects from all available standard and custom buffers. The user has the option to also manually input buffers that are close in value


Manual: manual buffer input from all available standard and custom values

Automatic Calibration



Selecting Buffers in Use, Standard or Custom (navigation guidelines)


In addition to selecting from 8 standard options, users can define 5 custom buffers to be used for calibration. **HI6221** automatically recognizes the closest buffer to the pH value being measured from all available (standard and custom) buffers.

To move buffers from **Available Standard Buffers** or **Available Custom Buffers** trays to **Buffers in Use** trays:

1. Tap .
2. Select **pH** Reading Parameter, and tap **Calibration** tab.
3. Tap **Edit**.



4. Tap to select from the Available Standard Buffers or Available Custom Buffers trays.
A rectangular outline highlights the buffer selected for transfer.
5. For standard values, tap  to move the selected buffer in the Buffers in Use column.
 displayed next to the buffer value, indicates calibration with standard buffer.
Repeat with up to 5 buffers.

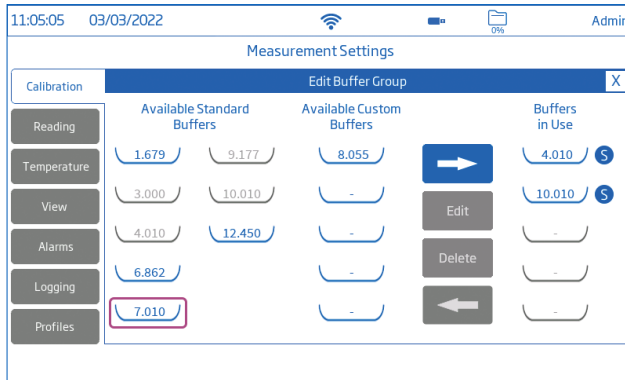


- For custom values, tap an empty tray to input a new value or an existing tray to edit. Follow the Editing Custom Buffers Values steps.


Editing Custom Buffer Values (navigation guidelines)

With **Calibration** tab selected:

- Tap **Edit** next to Buffer Group.
- Tap a custom buffer tray from the Available Custom Buffers column.
- Tap **Edit**.

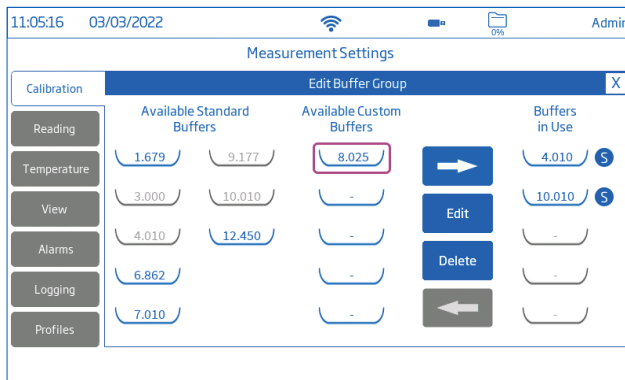

4. Use the numeric keypad to enter a value.

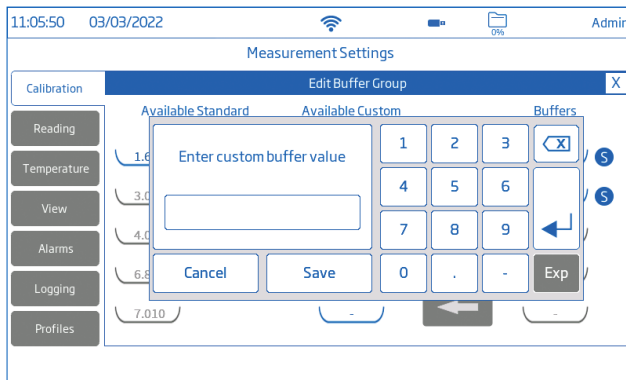

5. Tap or tap **Save** to confirm (Cancel to return without applying changes).

6. Tap on tray with newly-entered custom value.

A rectangular outline confirms that buffer can be transferred to Buffers in Use.

7. Use forward arrow to move custom buffer into Buffers in Use column.

Repeat with up to 5 buffers.

displayed next to the buffer value, indicates calibration with custom buffer.



Automatic pH Calibration Procedure

With the electrode and temperature sensor connected to the meter:

1. Select the correct buffer group or buffer value for calibration.
2. Select Manual Temperature source if calibration is done without a temperature sensor.
3. Remove the plastic protective cap from the probe and rinse the electrode with purified water.
4. Fill a rinse beaker 2/3 full with the first buffer solution.
5. Swirl the electrode and temperature sensor in the buffer solution.
6. Raise and lower the probe several times. Discard the solution.

7. Fill the calibration beaker 2/3 full with the first buffer solution.
8. Slowly place the electrode and temperature sensor in the selected buffer. Dislodge bubbles that may adhere to the sensors.

For most applications it is recommended to start with pH 7.01 buffer (or pH 6.86).

Use calibration buffers that bracket the samples pH.

For acidic samples it is recommended to use pH 4.01, 3.00, and/or 1.68 buffers.

For alkaline samples it is recommended to use pH 9.18, 10.01 and/or 12.45 buffers.

9. Tap Clear Calibration to start a fresh calibration and clear all previously used buffers. If using a new pH electrode it is recommended to tap Clear Calibration to clear all buffers and start new.
10. Rinse the electrode and temperature sensor in the buffer, place in the rinse beaker then calibration beaker.

A ➔ Buffer has been recognized. Waiting for reading to stabilize.

B ➔ Check the buffer value and use fresh buffer if:

- The buffer cannot be recognized.
- The current reading is outside of the acceptable window.
- The current buffer is generating a slope over the of acceptable window.
- Temperature is outside of the acceptable window.
- The current buffer is generating a low slope.
- The current buffer cannot be confirmed due to an inconsistency with the previous calibration (additionally, clear the old calibration to continue.)

C ➔ Check the buffer value and choose a new buffer if:

- The current buffer has already been accepted or is too close to a buffer that has been used.

Note: If probe's response time is slow, clean the probe then repeat the calibration.

Repeat procedure for a total of up to 5 calibration points.

11. Tap Save to update the calibration and return to the calibration setting screen. Tap the **Home** key (○) to return to measurement.

Semiautomatic Calibration

With Semiautomatic Calibration selected, users can confirm recognized buffer or change to another available buffer value by tapping the angle pointing arrow. The procedure is the same as Automatic Calibration.

Manual Calibration

With this option selected, the HI6221 uses from all available buffer values (standard and custom).

1. Tap **Calibration** tab.
2. Tap to select **Manual** calibration type.
3. Tap **Calibrate**.
4. Tap the angle forward pointing arrow on display to select correct buffer value.

10.2. RELATIVE mV CALIBRATION

The Rel. mV calibration or ORP calibration allows the user to:

- Perform a single point, custom calibration (Rel. mV).
- Restore the factory calibration (Clear Calibration).

The Oxidation-Reduction Potential (ORP), displayed in mV, is the voltage that results from the difference in potential between the platinum (or gold) ORP sensor and the silver/silver chloride reference electrode.

ORP values are not temperature compensated, although ORP values can change with temperature (e.g. reference electrode potential changes, sample equilibrium changes). It is important to report ORP values together with the reference electrode used and the temperature.

The inert noble metal ORP surface provides an electron-exchange site with the sample (or standard) and its surface. The electron exchange is typically very fast in well-poised solutions (e.g. standards), but may be lengthier in actual samples.

Calibration establishes a baseline that can be used as a comparison for future work. Calibration is used to compensate for changes due to contamination of the platinum surface and drift in the reference electrode.

A relative mV calibration can also be made to remove the voltage attributable to the Ag/AgCl reference electrode, to display the ORP versus a SHE (Standard Hydrogen Electrode).

This is an arithmetic correction and is correct only at the standard temperature. For example, [HI7022](#) ORP Test Solution reads 470 mV at 25 °C versus the Ag/AgCl reference. The ORP mV versus a SHE would be 675 mV (add 205 mV to the observed value).

Note: The user has to change the actual electrode to an ORP sensor and Parameter must be changed to Rel. mV for use with ORP electrodes. Suggested ORP models are [HI3133B](#), [HI4430B](#), or [HI3230B](#).

Please see Measurement Settings for details on configuration parameters and values.

When switching between Parameters (pH and mV, or Rel. mV), wait a few seconds to accommodate meter reconfiguration.

Rel. mV Calibration Procedure

1. Tap Calibrate and the meter will open a Rel. mV calibration screen.

10:07:11 03/03/2022 HI6221

Calibrate Rel.mV

Absolute mV: mV

Relative mV: mV

Press "Save" to update Rel mV.

Clear Calibration Cancel Save

- Place ORP electrode tip into a beaker of standard or a sample with known value.
HI7021 (ORP solution for platinum and gold electrodes) reads 240 mV at 25°C, **HI7022** (ORP test solution for platinum and gold electrodes) reads 470 mV at 25 °C.
- Tap the Relative mV box value.

- Tap Clear to remove previous values from the box.
- Use the keypad to enter the value of the standard.
- Tap Enter on keypad to confirm and enter the value.
- When a stable value is reached, tap Save.
 The meter returns to the Rel. mV calibration setup screen.
- Tap (Home key) to return to Measurement screen.

Clear calibration

- Tap **Clear** in calibration screen.
- The instrument prompts for confirmation.

11. MEASUREMENT

Options: Direct Readings, Direct/Autohold Readings

With **Direct** selected, sample measurements are displayed continuously.

With **Direct/Autohold** selected, reading is kept on display when measurement stability is reached. This option removes the subjective nature of stability as a measurement that has not reached equilibrium will not be used. After stability criteria is reached, the meter enters Direct/Autohold mode.

11.1. MEASUREMENT TIPS

- Connect the electrode to be used to the appropriate meter input. Make sure the electrode has been recently calibrated and is working correctly.
- Place electrode into the **HI764060** electrode holder for easy transfer in and out of containers during calibration, sample measurement, and storage.
- Rinse with purified water between buffers and / or samples.
- Blot (never rub) the glass pH sensor with a lint-free tissue between buffers and samples.
- To limit sample contamination, pour 2 beakers of buffers and samples. Use one beaker to rinse the sensor, and then use the second for measurement.
- Gently stir the test sample to ensure the sensor is measuring a representative sample.
- Open the fill hole cover and keep the fill solution topped off to permit the fill solution to flow through the ceramic junction and maintain a stable reference signal.

Note: Use the same size beaker and immersion depth for samples and buffers.


8. If measuring across a temperature gradient, allow the sensor to reach thermal equilibrium. If using manual temperature compensation input the sample temperature.
9. Once the reading indicates Stable, record measurement data.
10. Remove the electrodes from the sample, repeat steps 3, 4 and then place into the next rinse, then test sample.
11. Repeat the procedure for all samples. When all samples have been measured, rinse the pH electrode and replace storage cap with storage solution. Replace fill hole cover.

Note: When working without a temperature sensor, ensure that both calibration and measurements are done at the same temperature. This requires manual input of temperature value to allow the meter to perform buffer temperature correction.

11.2. DIRECT READINGS


From Measurement screen, tap  (Measurement Menu). Next:

- Tap to select from supported parameters.
- Tap **Direct** to select direct Reading Mode.
- Place the electrode tip and the temperature probe approximately 4 cm (1.5") into the sample to be measured. Allow time for the electrode to stabilize.
- Unstable status indicator on the screen until measurement is stabilized.
- The measured pH value is displayed on the LCD, together with GLP information and display preferences.

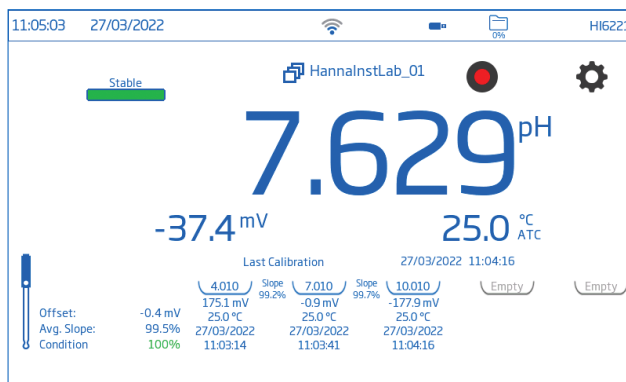


11.3. DIRECT / AUTOHOLD READINGS

From Measurement screen, tap  (Measurement Menu). Next:

- Tap to select from supported parameters.
- Tap **Direct/Autohold** to select direct/autohold Reading Mode.
- Place the electrode tip and the temperature probe approximately 4 cm (1.5") into the sample to be tested.
- The measured parameter value will be displayed on the LCD.
-  is displayed blinking until the stability criteria is reached.

- The measured value is kept on display and **Autohold** stops blinking.
- To return to direct Reading Mode, tap **pH** (pH icon).

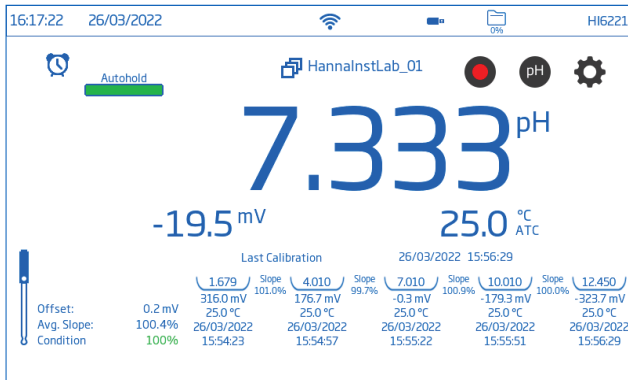

12. LOGGING

Three logging types are available: **Automatic**, **Manual**, and **Autohold**.

16:04:50 26/03/2022 Admin

Measurement Settings

Calibration

Reading

Temperature

View

Alarms

Logging

Profiles

Logging Type: Automatic Manual Autohold

Sampling Period: 180 min, 1 sec, 2 sec

File Name: Create 20220326_120026-relmV man-Lab1 05.csv

Log Note: Lab 1

Log Info 1: test

Log Info 2:


Automatic logging

- Readings are logged (tap **●**) at predefined time intervals. Sampling interval options range from 1 second to 180 minutes.
- Records are continuously added to it until the session stops.
- For each automatic logging session, a new log file is created.
- A complete set of GLP information including date, time, mode selection, temperature reading, and calibration information is stored with each log. User and log information e.g. company, address, sample details may also be included on the .CSV file.





Manual logging

- Readings are logged each time **●** is tapped.
- All manual readings are stored in a single log (i.e. records made on different days share the same log).






Autohold logging

- Readings are logged each time  is tapped and configured stability criteria is reached.
 - All Autohold readings are stored in a single log (i.e. records made on different days are logged in the same log).
- Note:** *Stability criteria can be set to Fast, Medium, or Accurate for all logging types.*






12.1. AUTOMATIC LOGGING

1. From Measurement screen, tap  (Measurement Menu).
2. Tap Reading tab and tap to select stability criteria (Accurate, Medium, or Fast).
3. Tap Logging tab and select Automatic logging type.
4. Scroll to select Sampling Period.
5. See option to define sample ID (name and prefix):
 - Tap Sample ID Prefix field to start editing.
 - Use the on-screen keypad to enter lot file name.
 - Tap Enter on keypad to save new name.
6. Tap  (Home key) to reenter Measurement screen.
7. From Measurement screen, tap  to start/stop logging.
8. During active logging, users can track and log notes.
To add a new log note:
 - Tap  (speech balloon symbol).
 - Use on-screen keypad to enter text.
 - Tap Enter on keypad to log entered note.
 Log Recall view, and .CSV log indicate the added log notes.

12.2. MANUAL LOGGING

1. From Measurement screen, tap  (Measurement Menu).
 2. Tap **Reading** tab and tap to select stability criteria (Accurate, Medium, or Fast).
- Note:** *Manual logging doesn't use this criteria for logging. Setting this is only for the user to note the stability of the reading.*
3. Tap **Logging** tab and select Manual logging type.
 4. See option to create file name:
 - Tap **Create**.
 - Use on-screen keypad to enter file name.
 - Tap  to save.
 5. See option to define sample ID (name and prefix).
 6. Tap  (Home key) to return to Measurement screen.
 7. From Measurement screen, tap  (manual logging symbol) to log data.
Data is logged every time symbol is tapped.
 8. See option to track and log notes.
 9. From Measurement screen, tap  to start/stop logging.

12.3. AUTOHOLD LOGGING

1. From Measurement screen, tap  (Measurement Menu).
2. Tap **Reading** tab to select stability criteria (Accurate, Medium, or Fast).
Note: Autohold logging uses this criteria for logging. Setting this will affect when data is recorded.
3. Tap for direct selection of Direct/Autohold reading mode.
4. Tap **Logging** tab and select Autohold logging type
5. Create a file name or have a file previously set up
6. Option to define sample ID (name and prefix)
 - Tap **Sample ID Prefix** field to start editing.
 - Use the on-screen keypad to enter lot file name.
 - Tap  to save.
 - Next, scroll to select Prefix value.
7. Tap  (**Home** key) to reenter Measurement screen.
8. From Measurement screen, tap  (Direct logging symbol) to start logging.
Active Autohold logging in progress is indicated by displayed  symbol.
Progress bar, top left corner, indicates progress status.
9. Once configured stability criteria is checked and conditions are met, data is logged.
The instrument prompts measurement screen, displayed in configured view.

CSV file format naming convention

To help identify measurement-specific data files within a data package (after download), logged files have the measurement unit automatically included in the file name (e.g. when reading and logging in pH Parameter, automatically logged files retain pH ID at the beginning of the file).

Manual or Autohold logged files retain the distinction between different reading modes in the file name. Users have the option to input file name:

- 20220329_085101-pH_auto.CSV
- 20220429_084105-mV_auto.CSV
- 20220309_095704-relmV_auto.CSV

13. MAINTENANCE & CONDITIONING

Electrode Maintenance

- Soak the pH bulb and reference junction in **HI70300** Storage Solution for a minimum of 30 minutes to refresh the electrode (before calibration).
- After prolonged storage or cleaning, calibrate the electrode.
- After use, rinse the electrode with purified water and blot excess moisture with a lint free tissue.
- Inspect all sensor connectors for corrosion and replace if necessary.

pH Sensor Maintenance

- Remove the sensor protective cap. Do not be alarmed if any salt deposits are present. This is normal with pH / ORP probes and they will disappear when rinsed with water.
- Shake down the probe as you would do with a clinical thermometer to eliminate any air bubbles inside the glass bulb.
- If the bulb and / or junction are dry, soak the electrode in [HI70300](#) Storage solution for at least 30 minutes.
- To ensure a quick response, the glass bulb and the junction should be kept moist and not allowed to dry. This can be achieved by storing the sensor with a few drops of [HI70300](#) Storage solution or pH 4.01 in the protective cap.

Note: *Never use distilled or deionized water to store electrode.*

Periodic Maintenance

- Inspect the electrode for any scratches or cracks. If any are present, replace the electrode.
- Inspect the cable. The connection cable must be intact.
- Rinse off any salt deposits with water.

pH Cleaning Procedure

1. Soak the sensor in [HI7061](#) Electrode cleaning solution for general use or application specific cleaning solution for 15 minutes.
2. Rinse with water.
3. Soak the electrode in [HI70300](#) Storage solution for at least 30 minutes, rinse with water and calibrate before using.

Protein, Inorganic, Oil, or Grease Cleaning Procedure

1. Soak the sensor in application specific electrode cleaning solution (i.e. [HI7073](#) Protein cleaning, [HI7074](#) Inorganic cleaning for 15 minutes or [HI7077](#) Oil and Fat cleaning solution).
2. Rinse the sensor with water.

Note: *After performing any of the cleaning procedures, rinse the electrode thoroughly with water and soak in [HI70300](#) Storage solution for at least 30 minutes before calibrating it.*

3. Soak the electrode in [HI70300](#) Storage solution for at least 1 hour, rinse with water, and calibrate before using.

General Cleaning of HI6221

The following steps outline the process to ensure users keep the benchtop clean and disinfected while limiting the risk of damage from unsuitable cleaners.

- Disinfect the screen using commercially available non-ammonia glass or disinfectant cleaner.
- Apply a small amount of cleaner directly to a microfiber or lint-free disposable cloth. Make sure the cloth is damp and not wet.
- Wipe the glass touch screen clean with the cloth. Do not apply cleaner directly to the interface.

14. ERROR MESSAGES

The instrument shows clear warning messages (refer to the instrument's on-display message area, bottom of the screen) when erroneous conditions appear, when measured values are outside the expected range, while logging, for invalid high/low temperature alarm value as well as invalid low/high mV Alarm value, isopotential point. The information below provides an explanation of the errors and warnings, and recommended action to be taken.

Displayed Message	Explanation & Recommended Action
"Temperature under/over range"	Temperature outside specified range. Verify the temperature probe is correctly connected to the meter. Replace probe if necessary.
"Under/over compensation range"	During pH calibration, the temperature is under/over the pH buffer compensation limit.
"pH over range"	Occurs when apparent pH value is more than 20.0 pH. Soak electrode in HI70300 Storage solution for at least 30 minutes.
"pH under range"	Occurs when apparent pH value is less than -2.0 pH. Soak electrode in HI70300 Storage solution for at least 30 minutes.
"pH out of calibration range"	Displayed when the measured value is outside calibration range.
"Rel. mV offset over/under range"	Outside range in the corresponding scale.
"mV under/over range"	
"Factory calibration expired"	Contact the Hanna technical support for the periodic factory calibration.

15. ACCESSORIES

pH BUFFER CALIBRATION SOLUTIONS

HI6016	Millesimal calibration buffer pH 1.679 (500 mL)
HI6003	Millesimal calibration buffer pH 3.000 (500 mL)
HI6004	Millesimal calibration buffer pH 4.010 (500 mL)
HI6068	Millesimal calibration buffer pH 6.862 (500 mL)
HI6007	Millesimal calibration buffer pH 7.010 (500 mL)
HI6010	Millesimal calibration buffer pH 10.010 (500 mL)
HI6124	Millesimal calibration buffer pH 12.450 (500 mL)
HI8004L	Buffer solution pH 4.01 (500 mL, FDA approved bottle)
HI8006L	Buffer solution pH 6.86 (500 mL, FDA approved bottle)
HI8007L	Buffer solution pH 7.01 (500 mL, FDA approved bottle)
HI8009L	Buffer solution pH 9.18 (500 mL, FDA approved bottle)
HI8010L	Buffer solution pH 10.01 (500 mL, FDA approved bottle)

ELECTRODE ELECTROLYTE REFILL SOLUTIONS

HI7071	3.5M KCl + AgCl Electrolyte for single junction electrodes, 4 pcs. (30 mL)
HI7072	1M KNO ₃ Electrolyte, 4 pcs. (30 mL)
HI7082	3.5M KCl Electrolyte for double junction electrodes, 4 pcs. (30 mL)
HI8071	3.5M KCl + AgCl Electrolyte in FDA approved bottle, for single junction electrodes, 4 pcs. (30 mL)
HI8072	1M KNO ₃ Electrolyte, 4 pcs. (30 mL, FDA approved bottle)
HI8082	3.5M KCl Electrolyte for double junction electrodes, 4 pcs. (30 mL, FDA approved bottle)
HI8093	1M KCl + AgCl Electrolyte, 4 pcs. (30 mL, FDA approved bottle)

ELECTRODE STORAGE SOLUTIONS

HI70300L	Storage solution (500 mL)
HI80300L	Storage solution (500 mL, FDA approved bottle)

ELECTRODE CLEANING SOLUTIONS

HI70000P	Electrode rinse sachet, 25 pcs. (20 mL)
HI7061L	General purpose solution (500 mL)
HI7073L	Protein cleaning solution (500 mL)
HI7074L	Inorganic substance cleaning solution (500 mL)
HI7077L	Oil and Fat cleaning solution (500 mL)
HI8061L	General purpose solution (500 mL, FDA approved bottle)
HI8073L	Protein cleaning solution (500 mL, FDA approved bottle)
HI8077L	Oil and fat cleaning solution (500 mL, FDA approved bottle)

OTHER ACCESSORIES

HI740036P	100 mL beaker (10 pcs.)
HI740037P	20 mL beaker (10 pcs.)
HI764060	Electrode holder
HI900946	115 Vac to 24 Vdc power adapter, US plug
HI900947	230 Vac to 24 Vdc power adapter, European plug
HI920016	USB type A to C cable

ELECTRODES

Electrode part numbers ending in **B** are supplied with a BNC connector and 1 m (3.3') cable.


Electrode part number ending in **Y** are supplied with a BNC + RCA connector

pH

HI1043B

Glass body, double junction, refillable, combination electrode


Application: strong acid or alkali

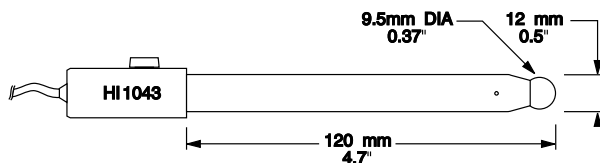

pH


HI1053B

Glass body, triple ceramic, conical shape, refillable, combination electrode
 Ideally suited for emulsions.

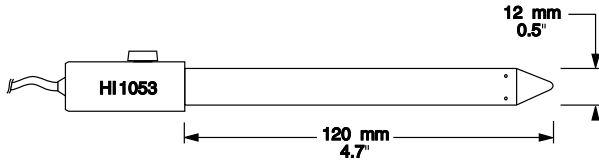


HI1083B

Glass body, micro, viscolene, non refillable, combination electrode
 Application: biotechnology, micro filtration

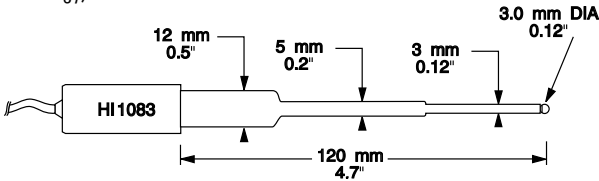


HI1131B

Glass body, refillable, double junction, combination electrode
 Application: general purpose

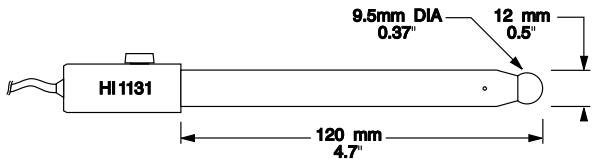

HI1330B

Glass body, semimicro, single junction, refillable, combination electrode
 Application: laboratory, vials

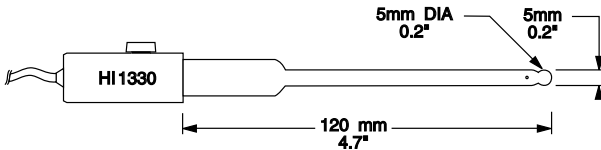


pH

HI1331B


Glass body, semimicro, single junction, refillable, combination electrode

Ideally suited for flasks.

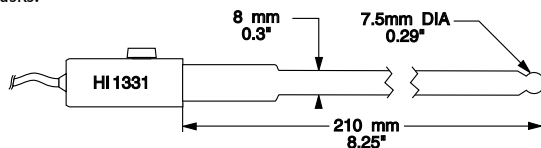**HI1230B**


Plastic body (PEI), double junction, gel filled, combination electrode

Application: general, field

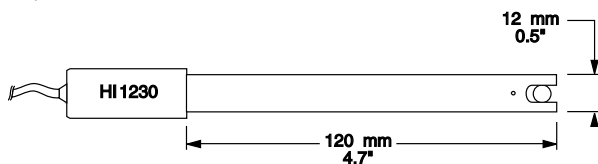**HI2031B**


Glass body, semimicro, conical, single junction, refillable, combination electrode

Application: semisolids

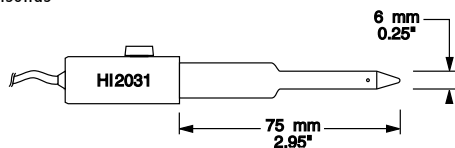**HI1332B**

Plastic body (PEI), double junction, refillable, combination electrode

Application: general purpose

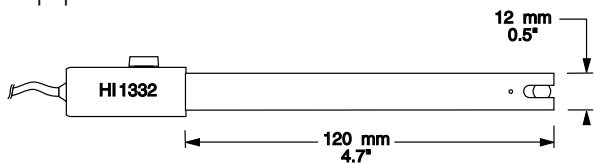


pH

HI1413B

Glass body, single junction, flat tip, viscolene, non refillable, combination electrode


Application: surface measurement

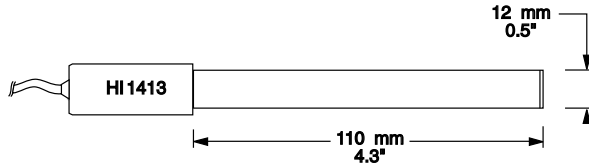

FC100B

Plastic body (PVDF), double junction, refillable, combination electrode


Application: general purpose for food industry

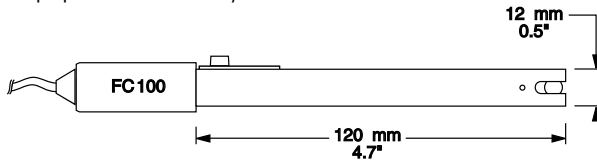

FC200B

Plastic body (PVDF), single junction, conical, viscolene, non refillable, combination electrode


Application: meat and cheese

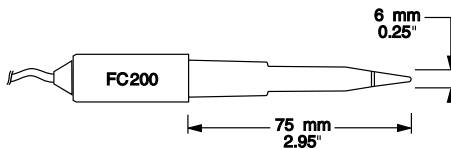

FC210B

Glass body, double junction, conical, viscolene, non refillable, combination electrode

Application: milk and yogurt

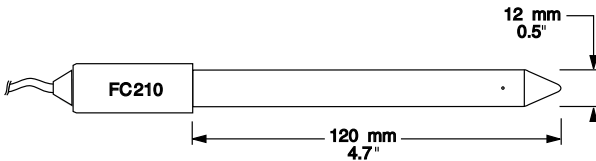


pH

FC220B

Glass body, triple ceramic, single junction, refillable, combination electrode

Application: food processing

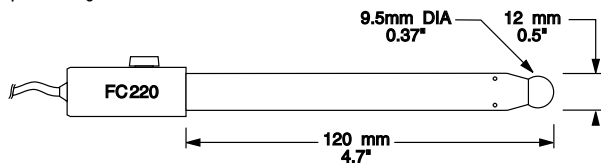


pH with 10K NTC thermistor

HI1131Y


Glass body, single ceramic frit, double junction, refillable, combination electrode

Application: general purpose

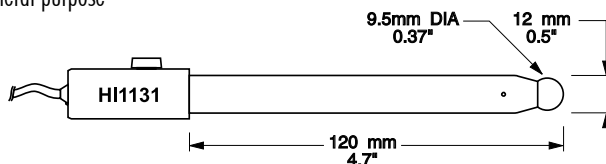**HI1230Y**

PEI body, single ceramic frit, double junction, combination electrode

Application: general purpose

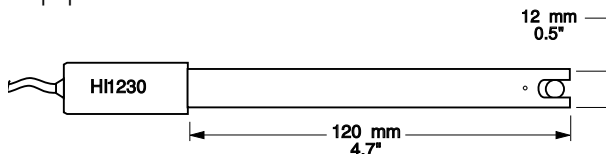**HI1048Y**

Glass body, CPS sleeve junction, combination electrode


Application: wine, must, and juice

ORP

HI3131B

Glass body, refillable, combination platinum electrode, ORP sensing pin

Application: titration

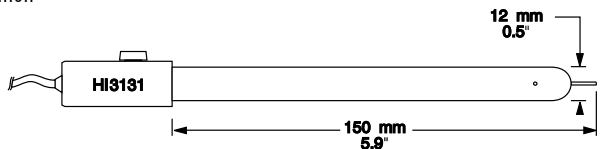


ORP

HI3230B

Plastic body (PEI), gel filled, combination platinum electrode, ORP sensing pin


Application: general purpose

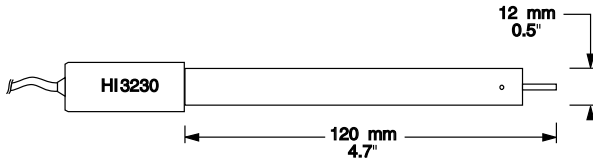

HI4430B

Plastic body (PEI), gel filled, combination gold electrode, ORP sensing pin

Application: general purpose

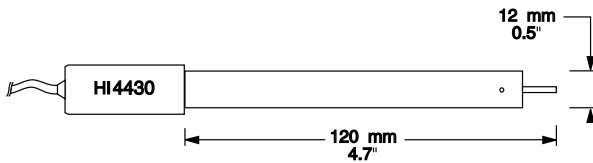

Extension cables for screw-type electrodes (screw to BNC adapter)



HI7855/1, 1 m (3.3') long

HI7855/3, 3 m (9.9') long

Connector and 3.0 mm (0.12") cable with BNC

Please refer to the Hanna Instruments general catalog for more electrodes with screw-type or BNC connectors.

16. ABBREVIATIONS

- ATC Automatic Temperature Compensation
- CSV Comma-Separated Values
- FTP File Transfer Protocol
- GLP Good Laboratory Practice
- IIS Internet Information Services
- MTC Manual Temperature Compensation
- NIST National Institute of Standards and Technology

CERTIFICATION

All Hanna® instruments conform to the CE European Directives and UK standards.



Disposal of Electrical & Electronic Equipment. The product should not be treated as household waste. Instead hand it over to the appropriate collection point for the recycling of electrical and electronic equipment which will conserve natural resources.

Ensuring proper product disposal prevents potential negative consequences for the environment and human health. For more information, contact your city, your local household waste disposal service, or the place of purchase.

RECOMMENDATIONS FOR USERS

Before using this product, make sure it is entirely suitable for your specific application and for the environment in which it is used. Any variation introduced by the user to the supplied equipment may degrade the meter's performance. For yours and the meter's safety do not use or store the meter in hazardous environments.

WARRANTY

HI6221 is warranted for two years against defects in workmanship and materials when used for its intended purpose and maintained according to instructions. Electrodes and probes are warranted for a period of six months. This warranty is limited to repair or replacement free of charge. Damage due to accidents, misuse, tampering or lack of prescribed maintenance is not covered.

If service is required, contact your local Hanna Instruments office. If under warranty, report the model number, date of purchase, serial number (see engraved on the bottom of the meter) and the nature of the problem. If the repair is not covered by the warranty, you will be notified of the charges incurred. If the meter is to be returned to Hanna Instruments, first obtain a Returned Goods Authorization number from the Technical Service department and then send it with shipping costs prepaid. When shipping any meter, make sure it is properly packed for complete protection.

REGULATORY NOTICES FOR THE WI-FI MODULE**United States (FCC)** FCC ID: 2ADHKATWINC1500.

This device complies with Part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) this device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

Canada (ISED) IC: 20266-WINC1500PB

HVIN: ATWINC1500-MR210PB

PMN: ATWINC1500-MR210PB

This device complies with Industry Canada's license exempt RSS standard(s). Operation is subject to the following two conditions: (1) This device may not cause interference, and (2) This device must accept any interference, including interference that may cause undesired operation of the device. Le présent appareil est conforme aux CNR d'Industrie Canada applicables aux appareils radio exempts de licence. L'exploitation est autorisée aux deux conditions suivantes: (1) l'appareil ne doit pas produire de brouillage, et (2) l'utilisateur de l'appareil doit accepter tout brouillage radioélectrique subi, même si le brouillage est susceptible d'en compromettre le fonctionnement.

Under Industry Canada regulations, this radio transmitter may only operate using an antenna of a type and maximum (or lesser) gain approved for the transmitter by Industry Canada. To reduce potential radio interference to other users, the antenna type and its gain should be so chosen that the equivalent isotropically radiated power (e.i.r.p.) is not more than that necessary for successful communication. Conformément à la réglementation d'Industrie Canada, le présent émetteur radio peut fonctionner avec une antenne d'un type et d'un gain maximal (ou inférieur) approuvé pour l'émetteur par Industrie Canada. Dans le but de réduire les risques de brouillage radioélectrique à l'intention des autres utilisateurs, il faut choisir le type d'antenne et son gain de sorte que la puissance isotrope rayonnée équivalente (p.i.r.e.) ne dépasse pas l'intensité nécessaire à l'établissement d'une communication satisfaisante.

Japan (MIC) 005-101762**South Korea (KCC)** R-CRM-mcp-WINC1510MR210P**Taiwan (NCC)** CCAN18LP0321T2

注意！依據 低功率電波輻射性電機管理辦法 第十二條 經型式認證合格之低功率射頻電機，非經許可，公司、商號或使用者均不得擅自變更頻率、加大功率或變更原設計之特性及功能。第十四條 低功率射頻電機之使用不得影響飛航安全及干擾合法通信；經發現有干擾現象時，應立即停用，並改善至無干擾時方得繼續使用。前項合法通信，指依電信規定作業之無線電信。低功率射頻電機須忍受合法通信或工業、科學及醫療用 電波輻射性 電機設備之干擾。

China (SRRC) CMIIT ID: 2018DJ1305**ANATEL** 08497-18-08759

Note: FCC information is marked on the back of the device.