

# IKA

designed for scientists

**MICROSTAR digital**



### EU Declaration of conformity

We declare under our sole responsibility that this product corresponds to the directives 2014/35/EU, 2006/42/EC, 2014/30/EU and 2011/65/EU and conforms with the following standards or normative documents: EN 61010-1, EN 61010-1-2-051, EN 61326-1, EN 60529 and EN ISO 12100.

A copy of the complete EU Declaration of conformity can be requested at [sales@ika.com](mailto:sales@ika.com).

## 8

### /// DEVICE SETUP

- › MICROSTAR digital . . . . . 8
- › What you should watch out for . . . . . 9

## 10

### /// SAFETY INSTRUCTIONS

- › Explication of warning symbols . . . . . 10
- › General information . . . . . 11
- › Device setup . . . . . 12
- › Working with the device . . . . . 13
- › Accessories . . . . . 15
- › Power supply / Switching off the device . . . . . 15
- › Disposal . . . . . 15

## 16

### /// INTENDED USE

- › Basics . . . . . 16

## 17

### /// UNPACKING

- › Scope of Delivery . . . . . 17

## 19

### /// USEFUL INFORMATION

- › Stirrer . . . . . 19

## 19

### /// SPEED

- › Speed – normal operation . . . . . 19
- › Speed – overload operation . . . . . 19
- › Output shaft . . . . . 20

## 21

### /// OPERATOR PANEL AND DISPLAY

- › Operation . . . . . 21

## 22

### /// ASSEMBLY

- › Assembling the extension arm to the overhead stirrer . . . . 22
- › Assembling the overhead stirrer to the stand . . . . . 23
- › Assembling the stirring element using the chuck . . . . . 23
- › Assembling the stirring shaft protector . . . . . 24
- › Assembling the mixing vessel to the stand . . . . . 24

## 25

### /// COMMISSIONING

- › Switching on . . . . . 25

## 26

### /// MAINTENANCE AND CLEANING

- › Cleaning . . . . . 26
- › Spare parts order . . . . . 27
- › Repair . . . . . 27

## 28

### /// ERROR CODES

- › Troubleshooting correctly . . . . . 28

## 29

### /// WARRANTY

- › Regulations . . . . . 29

## 29

### /// ACCESSORIES

- › An overview . . . . . 29

## 30

### /// PERMITTED IKA STIRRER TOOLS

- › An overview . . . . . 30

## 31

### /// TECHNICAL DATA

- › MICROSTAR digital in detail . . . . . 31

# Device setup

/// MICROSTAR digital



1	Operator panel and display
2	Chuck
3	Extension arm
4	Power socket
5	USB interface
6	Stirring shaft cap

/// What you should watch out for



Attention! (X)

# Safety instructions

/// Explication of warning symbols



Indicates an (extremely) hazardous situation, which, if not avoided, **will result in death, serious injury.**



Indicates a hazardous situation, which, if not avoided, **can result in death, serious injury.**



Indicates a potentially hazardous situation, which, if not avoided, **can result in injury.**



Indicates practices which, if not avoided, **can result in equipment damage.**

/// General information

- › **Read the operating instructions in full before starting up and follow the safety instructions.**
- › Keep the operating instructions in a place where it can be accessed by everyone.
- › Ensure that only trained staff work with the device.
- › Follow the safety instructions, guidelines, occupational health and safety and accident prevention regulations.

## **Danger! (X)**

Please pay attention to the dangerous parts of the equipment in device setup. Beware of the risk of:

- › flammable materials
- › glass breakage as a result of mechanical stirring power

## **Caution! (X)**

Wear your personal protective equipment in accordance with the hazard category of the medium to be processed, there is a risk of:

- › splashing of liquids
- › projectile parts
- › body parts, hair, clothing and jewelry getting caught

**The device must only be used in a technically perfect condition.**

## /// Device setup

### **Danger! (X)**

Users must make sure that the standby key of the IKA device can be accessed immediately, directly and without risk at any time. If installation or positioning cannot ensure this access at all times, an additional **EMERGENCY STOP** switch that can be easily accessed must be installed in the work area.

### **Warning! (!)**

Ensure stable assembly. The vessel used for stirring must be secured. Use stirring shaft protective equipment!

- › **Set up the stand in a spacious area on an even, stable, clean, non-slip, dry and fireproof surface.**
- › **Remove the chuck key from the chuck before turning on the device.**
- › Place the power supply outside the working area of the device.
- › Avoid knocking and impacting on the lower end of the shaft and the chuck gear teeth. Even minor, invisible damage can lead to imbalance and uneven shaft action.
- › All screw connections must be properly tightened.
- › The high torque developed by the device requires particular care in the choice of stand, cross sleeve and anti-rotation element for the agitating vessel.

## /// Working with the device

### **Danger! (X)**

- › Do not use the device in explosive atmospheres, it is not EX-protected.
- › With substances capable of forming an explosive mixture, appropriate safety measures must be applied, e.g. working under a fume hood.
- › To avoid body injury and property damage, observe the relevant safety and accident prevention measures when processing hazardous materials.
- › The device is not suitable for hand-held operation.
- › Do not touch rotating parts during operation!

### **Warning! (!)**

Pathogenic materials must only be processed in closed vessels under a suitable fume hood. If you have any questions, please contact IKA application support.

The operation of a free rotating shaft end is prohibited. Therefore, for safety reason, only insert through the stirring tool over the upper edge of housing at standstill.

### **Caution! (Z)**

Make certain that the unit is set at the lowest speed before commissioning; otherwise, the unit will begin running at the speed set in last operation. Gradually increase the speed. Please observe the max. permitted speed for the stirring element. Never set higher speed.

**Covers or parts that can be removed from the device without tools must later be refitted to ensure safe operation. This will prevent the infiltration of foreign objects, liquids and other contaminants.**

- › Imbalance of the output shaft, the chuck and in particular the stirring tools can lead to uncontrolled resonant vibrational behavior of the device and the whole assembly. Glass apparatus and stirrer containers can be damaged or shattered by this. It can cause injury to the operator, also can damage the rotating stirring tool. In this case exchange the stirring tool for one without imbalance or remedy the cause of the imbalance. If there is still imbalance, return it to the dealer or the manufacturer along with a description of the fault.
- › There may be electrostatic activity between the medium and the output shaft which could cause a direct danger.
- › Never operate the device with the stirrer tools rotating freely. Ensure that parts of the body, hair, jewelry or items of clothing cannot be trapped by the rotating parts.
- › Pay attention when setting the speed to any imbalance of the stirrer tools and possible spraying of the medium to be stirred.
- › Ensure that the stand does not start to move.
- › Only process media that will not react dangerously to the extra energy produced through processing. This also applies to any extra energy produced in other ways, e.g. through light irradiation.

**Reduce the speed if:**

- › the medium splashes out of the vessel because the speed is too high,
- › the device is not running smoothly,
- › the device begins to move around because of dynamic forces,
- › an error occurs.

### /// Accessories

- › Protect the device and accessories from bumping and impacting.
- › Check the device and accessories beforehand for damage each time when you use them. Do not use damaged components.
- › Safe operation is only guaranteed with the accessories described in the "Accessories" section.
- › Must disconnect the power before changing stirring element and fitting allowed accessories.

### /// Power supply / Switching off the device

**If the device is operated too long in overload or if the ambient temperature is too high, the device switches off permanently.**

- › Disconnecting the device from the power outlet only works by removing the main cord from the socket.
- › The device must only be operated with the original power supply unit.
- › The power supply comes with interchangeable plug adapters for different countries so make sure the appropriate adapter is used.
- › The outlet for the power supply must be easily accessible.
- › After an interruption in the power supply during a stirring process, the device does not restart automatically.
- › The device must only be opened by trained technicians, even during repair. The device must be unplugged from the power supply before opening. Live parts inside the device may still be live for some time after unplugging from the power supply.

### /// Disposal

The device must be disposed of in accordance with national regulations.



# Intended use

/// Basics

## Use

- › For mixing / stirring liquids from low to medium viscosities with various stirring tools.
- › **Stand device** (chuck points down)

## Range of use (indoor use only)

- › Laboratories
- › Pharmacies
- › Universities
- › Schools

The device is suitable for use in all areas (EMC class A and B).

## The safety of the user cannot be guaranteed:

- › if the device is operated with accessories that are not supplied or recommended by the manufacturer.
- › if the device is operated improperly or contrary to the manufacture's specifications.
- › if the device or the printed circuit board are modified by third parties.


# Unpacking

/// Scope of Delivery


Unpack the device carefully. **Any damage should be notified immediately to the shipping agent (post office, railway network or logistics company).**

## Scope of Delivery

- › MICROSTAR digital overhead stirrer
- › power supply (with exchangeable adapters)
- › extension arm
- › hexagonal socket screw
- › hexagon socket offset screw key
- › shaft protector R 300 (with 2 fasten screws)
- › chuck key
- › USB cable
- › user guide
- › warranty card

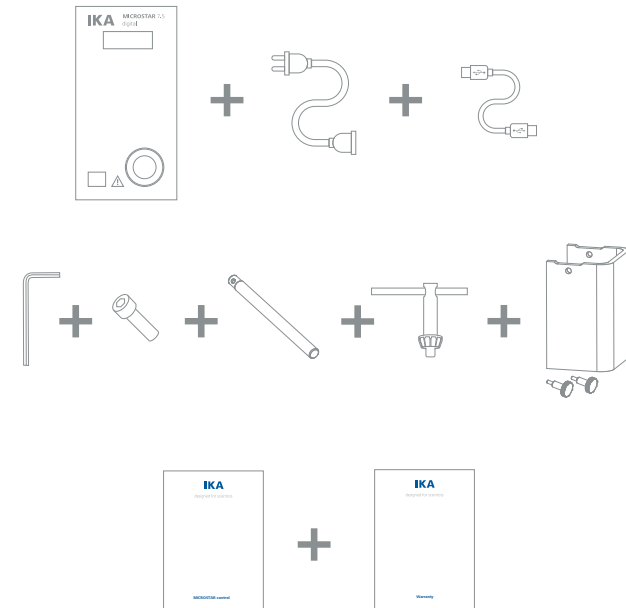

### Power supply unit (with exchangeable adapters)

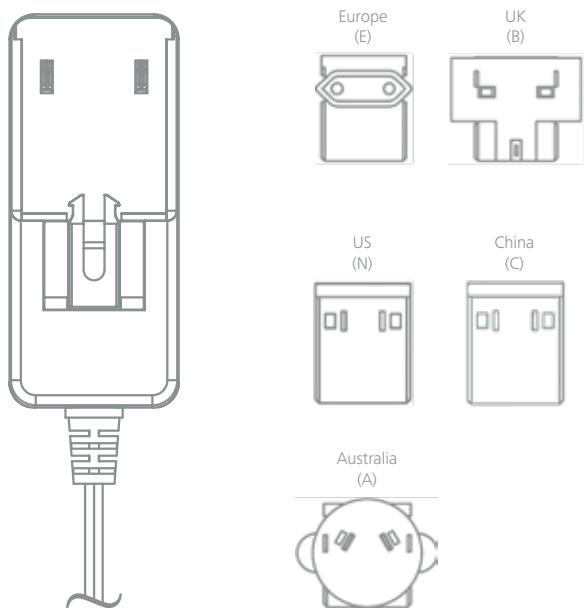

Schematics of device and power supply.

## Useful information

### /// Stirrer

The stirring device is suitable for continuous operation. The motor current is limited electronically. The device has an anti-stall and anti-overload system. If a fault occurs, a safety circuit immediately switches off the motor permanently. The device starts with the last settings made.

## Speed

### /// Speed – normal operation

#### Speed - regulated (no variation in speed):

The speed is monitored and regulated by processor controlled. The target speed is constantly compared with the actual rotation speed value of the output shaft and variations corrected. This guarantees a constant speed even if the viscosity of the substance being stirred changes.

Fluctuations in mains voltage within the permitted tolerance range have no effect on the quality of regulation and constancy of speed.

The speed is set using the front knob. During normal operations the speed value on the display corresponds to the speed of the output shaft in revolutions per minute (rpm).

### /// Speed – overload operation

When solid or semi-viscous substances are added, the stirrer can be run for a brief period at 130% its rated power. When running in the overload range (for instance if the viscosity has increased at a particular stage of the process) the speed will reduce to a degree sufficient to keep the torque on the stirrer shaft within the rated torque of the device.

### Overload status 1

The device is already running within the overload range, however, the actual speed does not match the set speed. This condition is maintained as long as neither the motor current nor the device temperature exceeds their permissible limit value. Display symbol: blinking of the target speed.

### Overload status 2

The device stop at a load above 130 % of the nominal torque.  
Message in the display (see "Error codes" section).

## /// Output shaft

### Caution! (⚠)

Please see section "Safety instructions"!

The clamping chuck and output shaft permit clamping IKA recommend stirrer tools (see section "Permitted IKA Stirrer tools"). The output shaft is designed as a hollow shaft and the opening on the top side of the housing is closed with a plastic cover. When the stirrer cover is opened, it is possible for stirring shaft to be pushed out over the top edge of the housing at standstill, e.g. during changing container.

For safety reason, the stirrer cover must be pushed back into the opening of the housing so that it is properly closed. This is the only way to ensure that working with the unit is safe and that media cannot enter the device.

## Operator panel and display


### /// Operation



<b>A</b>	Standby key	Device switches on / enters standby (no disconnection from the power supply network).
<b>B</b>	Display	Display the speed value.
<b>C</b>	Control knob (rotating/pressing)	Set the speed by rotating. Start / stop the stirrer function by pressing.


# Assembly

/// Assembling the extension arm to the overhead stirrer

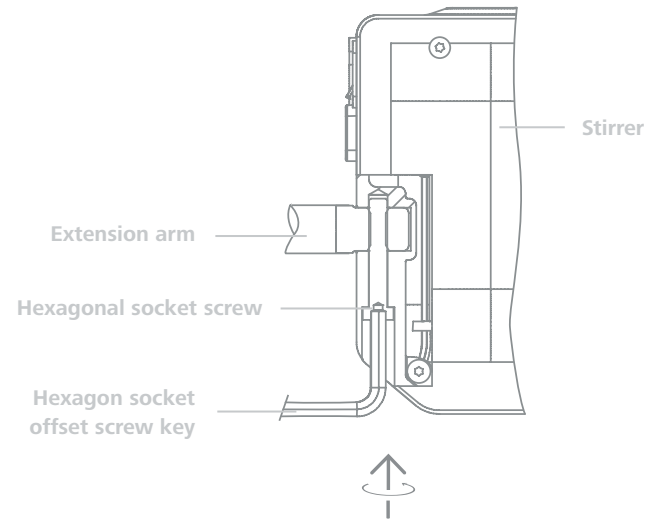


Ensure that the extension arm is fitted securely. Vibration may cause the screw to become loose. It is therefore necessary for safe use to regularly check that the extension arm is attached securely. Tighten the hexagonal bolt as required.

/// Assembling the overhead stirrer to the stand

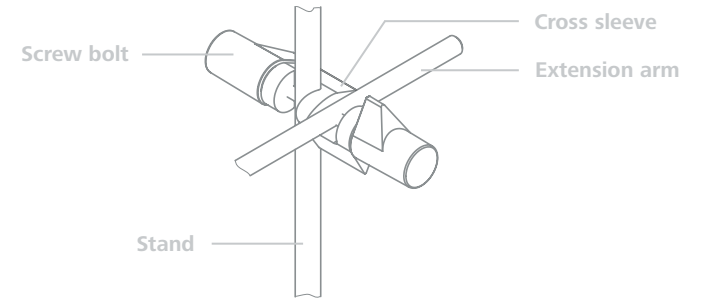

Check that the stirrer is held in position firmly prior to each use and also at regular intervals. The position of the stirrer must only be adjusted when the equipment is stationary and the power supply is disconnected.


/// Assembling the stirring element using the chuck

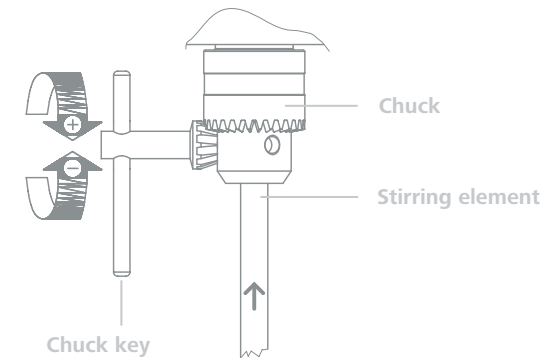

### Warning! (!)

The stirring element must only be changed when the equipment is stationary and the power supply is disconnected.

### /// Assembling the stirring shaft protector

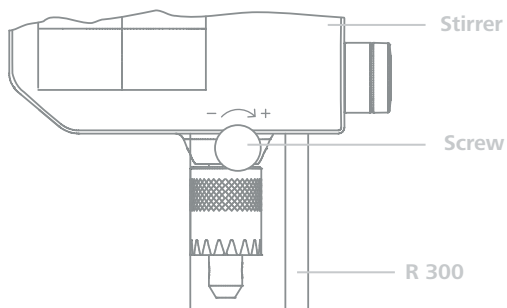

### /// Securing the mixing vessel to the stand



## Commissioning

### /// Start-up

#### **Secure the device to a stable stand with a cross sleeve.**

The stirring vessel must always be securely fixed for safety reasons. You must also ensure that the mounting device (stand) is set up in such a way that it is not liable to topple and does not start to move during the stirring procedure.

If these conditions have been met, the machine is ready for operation when the mains plug is plugged in. If these conditions are not met, safe operation is not guaranteed and the machine could be damaged.

Observe the ambient conditions (temperature, humidity, etc.) listed under "Technical Data".

#### **The AC adapter is suitable for 100 VAC to 240 VAC.**

The exchangeable adapter for the relevant country must be attached before the AC adapter is plugged into the mains socket.

#### **Switching on/off**

1. After connecting the power to the device or touching the standby key **(A)** more than 1 second, the device is switched on. Following screens appear:

8.8.8.8. — Self test screen

7.5d — Device identification

1.0.1 — Software version

2. After that, the following screen appears automatically.

0 — Last speed setting

3. Then, the device is ready for operation.

4. After switching off the device by touching the standby key **(A)** more than 1 second, following screen appears:

— Standby LED

### Setting speed

- › Ensure the speed set is suitable for the test medium selected. If in doubt, set the speed to the lowest speed (counterclockwise direction) by rotating the control knob **(C)**. Press the control knob **(C)** to start or stop the stirring. During running, the standby LED blinks to indicate the running status.

## Maintenance and cleaning

### /// Cleaning

The device is maintenance-free. It is only subject to the natural wear and tear of components and their statistical failure rate.

For cleaning disconnect the main plug!

Use only cleaning agents which have been approved by IKA to clean IKA devices.

Dirt	Cleaning agent
Dye	isopropyl alcohol
Construction material	water containing tenside / isopropyl alcohol
Cosmetics	water containing tenside / isopropyl alcohol
Foodstuffs	water containing tenside
Fuel	water containing tenside

For materials which are not listed, please request information from IKA application support. Wear protective gloves during cleaning the devices. Electrical devices may not be placed in the cleansing agent for the purpose of cleaning. Do not allow moisture to get into the device when cleaning. Before using another than the recommended method for cleaning or decontamination, the user must ascertain with IKA that this method does not destroy the device.

### /// Spare parts order

When ordering spare parts, please give:

- › machine type
- › serial number, see type plate
- › item and designation of the spare part, see [www.ika.com](http://www.ika.com), spare parts diagram and spare parts list
- › software version

### /// Repair

**Please send in device for repair only after it has been cleaned and is free from any materials which may constitute a health hazard.**

For repair, please request the “Decontamination Certificate” form IKA or use the download printout of it from IKA website: [www.ika.com](http://www.ika.com).

If you require servicing, return the device in its original packaging. Storage packaging is not sufficient. Please also use suitable transport packaging.

## Error codes

### /// Troubleshooting correctly

If an error occurs, the fault is shown by an error code on the screen.

Proceed as follows in such cases:

- › Disconnect the device from the power supply.
- › Carry out corrective measures.
- › Restart device.

#### Error code | Cause | Effect | Solution

##### E 2

Cause	› hardware driving error
Effect	› motor off
Solution	› contact the service department

##### E 3

Cause	› temperature inside of the device is too high
Effect	› motor off
Solution	› switch off the device and allow it cool down

##### E 4

Cause	› motor blockage or overload
Effect	› motor off
Solutions	› disconnect the device from the power supply › decrease the load on the motor and restart device again

##### E 8

Cause	› speed sensor fault or overload
Effect	› motor off
Solution	› disconnect the device from the power supply

**If the actions described fails to resolve the fault or another error code is displayed then take one of the following steps:**

- › Contact the service department.
- › Send the device for repair, including a short description of the fault.

## Warranty

### /// Regulations

In accordance with IKA warranty conditions, the warranty period is 24 months.

For claims under the warranty please contact your local dealer. You may also send the machine direct to our factory, enclosing the delivery invoice and giving reasons for the claim. You will be liable for freight costs.

The warranty does not cover worn out parts, nor does it apply to faults resulting from improper use, insufficient care or maintenance not carried out in accordance with the instructions in this operating manual.

## Accessories

### /// An overview

#### General accessories

- › **R 1825** Plate stand
- › **R 1826** Plate stand
- › **R 1827** Plate stand
- › **R 182** Cross sleeve
- › **RH 3** Strap clamp
- › **R 300** Stirring shaft protection (with 2 screws)
- › **FK 1** Flexible coupling
- › **USB 2.0 cable A – micro B**

See more accessories on [www.ika.com](http://www.ika.com).

# Permitted IKA stirrer tools

/// An overview

## Propeller stirrer

- › **R 1342** max. speed (rpm) ≤ 2000
- › **R 1381** max. speed (rpm) ≤ 2000
- › **R 1382** max. speed (rpm) ≤ 2000

## Propeller stirrer, PTFE

- › **R 1389** max. speed (rpm) ≤ 800

## Turbine stirrer

- › **R 1311** max. speed (rpm) ≤ 2000
- › **R 1312** max. speed (rpm) ≤ 2000

## Dissolver stirrer

- › **R 1300** max. speed (rpm) ≤ 2000
- › **R 1303** max. speed (rpm) ≤ 2000

## Centrifugal stirrer

- › **R 1352** max. speed (rpm) ≤ 2000

## Anchor stirrer

- › **R 1330** max. speed (rpm) ≤ 1000

See more permitted stirrer tools on [www.ika.com](http://www.ika.com).

# Technical data

/// MICROSTAR digital in detail

## Technical data MICROSTAR digital

	MICROSTAR		
	7.5 digital	15 digital	30 digital
Speed range under nominal load	0 / 50 ... 2000 rpm	0 / 50 ... 1000 rpm	0 / 50 ... 500 rpm
Speed adjustment	Stepless		
Speed display	LED		
Speed setting accuracy	± 1 rpm		
Speed measurement deviation	Speed < 300 rpm: ± 3 rpm, Speed > 300 rpm: ± 1 %		
Max. torque at stirrer shaft	7.5 Ncm	15 Ncm	30 Ncm
Max. stirring quantity (water)	5 l	10 l	20 l
Max. viscosity	4000 mPa·s	8000 mPa·s	20000 mPa·s
Interface	USB		
Permitted on time	100 %		
Nominal voltage	24 VDC		
Max. current	1300 mA		
Max. input power	32 W		
Max. output power at stirring shaft	15.7 W		
IP code according to EN 60529	IP 54		
Contamination level	2		
Protection at overload	motor current limitation		
Ambient temperature	5 ... 40 °C		
Ambient humidity (rel.)	80 %		
Drive	Brushless DC-Motor		
Clamping chuck-clamping range	0.5 ... 8 mm		
Hollow shaft internal diameter	8.5 mm		
Extension arm (Ø × L)	13 × 160 mm		
Dimensions (W × D × H) (without extension arm)	60 × 126 × 173 mm		
Weight (with extension arm and clamping chuck)	1.18 kg	1.26 kg	1.26 kg
Operation at a terrestrial altitude	max. 2000 m		



---

**Power supply**

---

	100 ... 240 VAC
	1 A
Input	50 / 60 Hz
	24 VDC
Output	36 W LPS (Limited Power Source)
Protection class	II (double insulated )

---



designed for scientists

---

**IKA-Werke GmbH & Co. KG**

Janke & Kunkel-Straße 10, 79219 Staufen, Germany  
Phone: +49 7633 831-0, Fax: +49 7633 831-98  
eMail: sales@ika.de

---

**USA**

IKA Works, Inc.  
Phone: +1 910 452-7059  
eMail: sales@ika.net

**KOREA**

IKA Korea Ltd.  
Phone: +82 2 2136 6800  
eMail: info@ika.kr

**BRAZIL**

IKA Brasil  
Phone: +55 19 3772 9600  
eMail: sales@ika.net.br

**MALAYSIA**

IKA Works (Asia) Sdn Bhd  
Phone: +60 3 6099-5666  
eMail: sales.lab@ika.my

**CHINA**

IKA Works Guangzhou  
Phone: +86 20 8222 6771  
eMail: info@ika.cn

**POLAND**

IKA Poland Sp. z o.o.  
Phone: +48 22 201 99 79  
eMail: sales.poland@ika.com

**JAPAN**

IKA Japan K.K.  
Phone: +81 6 6730 6781  
eMail: info\_japan@ika.ne.jp

**INDIA**

IKA India Private Limited  
Phone: +91 80 26253 900  
eMail: info@ika.in

**ENGLAND**

IKA England LTD.  
Phone: +44 1865 986 162  
eMail: sales.english@ika.com

---

Discover and order the fascinating products of IKA online:

**[www.ika.com](http://www.ika.com)**

---



---

Technical specifications may be changed without prior notice.