

Secura®

Benefits

- Top Performance
- Intuitive Operation
- Ergonomic Draft Shield
- Automatic Internal Adjustment
- Real-Time Level Support



Product Information

Secura[®] gives you the security and peace of mind of knowing that you have done everything right. Besides providing highly accurate weighing results and operating convenience, Secura[®] also features built-in protection systems for complete reliability and regulatory compliance – the safe and secure way.

Real-time guidance prompts for leveling, automatic internal adjustment and 100% traceable, clear documentation with sample and batch identifiers make your lab work more efficient.

First, the new operating concept of Secura[®] will noticeably ease your daily workload during weighing and, second, its APC function – Advanced Pharma Compliance – will relieve you from tedious and time-consuming documentation and monitoring tasks.

Technical Specifications

AC Adapter		Ambient Conditions					
Sartorius AC adaptor module	6971790 with interchangeable country-specific plug-in AC	The specifications apply when the following ambient conditions are in place:					
	adaptors	Environment	for indoor use only				
Primary	100 – 240 V~, –10% +10%, 50 – 60 Hz, 0.2 A	Ambient temperature*	+10 °C to +30 °C				
Secondary	15 V DC, ± 5%, 530 mA (max.)	Operational capacity	guaranteed between +5 °C and +45 °C				
	8 Watt (max.): 0 to +40 °C and 15 V DC, ± 5%, 330 mA (max.)	Storage and shipping	–10 °C to +60 °C				
	5 Watt (max.): 0 to $+50 ^{\circ}\text{C}$	Elevation	up to 3000 m above sea level				
Other data	protection class II, in accordance with EN IEC 60950-1 up to 3000 m above sea level; IP40 as per EN IEC 60529	Relative humidity**	15% to 80% for temperatures up to 31 °C; non-condensing, decreasing linearly to 50% relative humidity at 40 °C and 20% at 50 °C				
Balance		Safety of electrical equipment	in accordance with EN 61010-1/ IEC 61010-1. Safety requirements for electrical equipment for mea				
Power supply	only via Sartorius AC adaptor module 6971790		surement, control, and laboratory use – Part 1: General requirements				
Input voltage	12.0 18.0 V DC	Electromagnetic	in accordance with EN 61326-1/				
Power consumption	2.0 W (typically) 4.5 W (typically), only for 225D-1x, 125-1x and 324-1x	compatibility	IEC 61326-1. Electrical equipment for measurement, control, and laboratory use – EMC requirements – Part 1: General requirements				
		Defined immunity to interference	Suitable for use in industrial areas				
		Interference emission	Class B (suitable for use in residential areas and areas that are connected to a low voltage network that also supplies residential buildings). The device can therefore be				

Balances verified for use in legal metrology comply with the requirements of Council Directive 2009/23/EC, EN 45501:1992, and OIML R76:2006.

used in both areas.

For balances verified for use in legal metrology in accordance with EU requirements, refer to the information on the balance.
 ** For balances verified for use in legal metrology in accordance with

EU requirements, the legal regulations apply.

Standard Equipment	
APC Features	 Monitoring of compliance with the USP minimum sample weight limits - SQmin Password protection of set-up settings Fully automatic temperature- and time-controlled internal calibration and adjustment - isoCAL Temporary blockage of data transfer to a printer or a com- puter when uncertain weighing results are detected, such as a result is below the USP minimum sample weight limit, the balance is not level or isoCAL calibration adjustment needs to be per- formed Storage of all data of calibration procedures - Cal Audit Trail
Safety Level	Three configurable levels of security
Levelling	Intelligent, optoelectronic leveling sensor with alarm function and interactive user guidance for reliable leveling
Calibration	Internal calibration isoCAL, External calibration
Selectable weight units ¹⁾	Gram, kilogram, carat, pound, ounce, troy ounce, Hong Kong tael, Singapore tael, Taiwan tael, grain, pennyweights, milligram, parts per pound, China tael, mommes, Austrian carat, tola, baht, mesghal and Newton
Interface	 mini USB Automatic recognition of Sartorius printer models YDP30 or YDP40 Direct data transfer to Microsoft[®] Windows programs Programmable interval for data output Data transfer protocols SBI, xBPI, table format, text format
Display	Touch screen with Sartorius graphical user interface

Standard Equipment	
Standard built-in applications	Weighing, Density, Percentage, Checkweighing, Peak Hold, Counting, Unstable Conditions Animal weighing
Special built-in lab applications	Mixing, Components, Statistics, Conversion
Languages	English, French, German, Hungarian, Italian, Polish, Portuguese, Russian, Spanish, Turkish, Chinese, Japanese, Korean
Protection	 Chemical resistant finish of the top housing Glass parts of the draft shield are coated to reduce electrostatic influences In-use cover Dust cover for balances with draft shield
Anti-theft lock	Kensington lock and lockdown capability for cable or chain

¹⁾ Limited for verified models



Standard Models

Model		26-1x ¹⁾	225D-1x ¹⁾	125-1x ¹⁾	324-1x ¹⁾
Design		1	2	2	2
Weighing capacity	g	21	60 120 220	60 120	320
Readability	mg	0.002	0.01 0.01 0.1	0.01 0.01	0.1
Repeatability (standard deviation)	mg	0.004	0.03 0.04 0.07	0.03 0.04	0.1
Repeatability (standard deviation), typical	mg	0.003	0.02 0.04 0.07	0.02 0.04	0.1
Linearity deviation	mg	0.01	0.1 0.1 0.2	0.1 0.1	0.3
Typical starting point of the operating range 2)	mg	4	25**	25**	160
Optimal starting point of the operating range ²⁾	mg	1.64*	8.2**	8.2**	82
Sensitivity drift between +10 °C and +30 °C	± ppm/K	1	1	1	1
Typical stabilization time	S	8	6 6 2	6 6	2
isoCAL: – Temperature change – Time interval	K h	1.5 4	1.5 4	1.5 4	1.5 4
Display result (depending on the set filter level)	S	0.2 0.4	0.2 0.4	0.2 0.4	0.2 0.2
Weighing pan size	mm	Ø 50	arnothing 80 (optional $arnothing$ 90)	arnothing 80 (optional $arnothing$ 90)	Ø 90
Weighing chamber height***	mm	218	218	218	218
Net weight, approx.	kg	8.0	7.8	7.8	7.9
IP protection class		IP43	IP43	IP43	IP43



In combination with glass draft shield YHK01SQP
 In combination with weighing pan, 80 mm, slotted YSP01SQP
 Upper edge of the weighing pan to the lower edge of the upper draft shield panel

¹⁾ Possible terms for country-specific models:

- x = S: Standard balances without country-specific additions
- x = SAR: Standard balances with country-specific additions for Argentina
- x = SJP: Standard balances with country-specific additions for Japan
 x = SKR: Standard balances with country-specific additions for South Korea
- According to USP (United States Pharmacopeia) Chapter 41, the optimal operating range is defined from 820d to maximum weighing capacity. 2) Depending on the installation location and environmental conditions, the value could be higher.

Model		224-1x ¹⁾	124-1x ¹⁾	1103-1x ¹⁾	613-1x ¹⁾	513-1x ¹⁾	313-1x ^{1]}	⁾ 213-1x ¹⁾	6102-1x ¹⁾
Design		3	3	4	4	4	4	4	5
Weighing capacity	g	220	120	1,100	610	510	310	210	6,100
Readability	mg	0.1	0.1	1	1	1	1	1	10
Repeatability (standard deviation)	mg	0.1	0.1	1	1	1	1	1	10
Linearity	mg	0.2	0.2	2	2	2	2	2	20
Typical starting point of the operating range ²⁾	g	0.12	0.12	1.5	1.5	1.5	1.5	1.5	12
Optimal starting point of the operating range ²⁾	g	0.082	0.082	0.82	0.82	0.82	0.82	0.82	8.2
Sensitivity drift between +10 to +30°C	± ppm/K	1.5	1.5	1.5	2	2	2	2	2
Typical stabilization time	S	2	2	1.5	1	1	1	1	1
isoCAL Settings: – temperature change – time interval	K h	1.5 4	1.5 4	1.5 4	2 6	2 6	2 6	2 6	2 6
Display result (depending on the filter level)	S	0.2	0.2	0.1 0.2	0.1 0.2	0.1 0.2	0.1 0.2	0.1 0.2	0.1 0.2
Weighing pan size	mm	Ø 90	Ø 90	Ø 120	Ø 120	Ø 120	Ø 120	Ø 120	Ø 180
Weighing chamber height***	mm	209	209	209	209	209	209	209	-
Net weight, approx.	kg	5.1	5.1	5.9	5.1	5.1	5.1	5.1	5.2
Model		5102-1x ¹⁾	3102-1x	¹⁾ 2102-1	x ¹⁾ 1102	-1x ¹⁾ 612	2-1x ¹⁾	6101-1x ¹⁾	3101-1x ¹⁾
Model Design		5102-1x¹⁾	3102-1 x	¹⁾ 2102-1 5	x¹⁾ 1102 5	-1x¹⁾ 612 5		6101-1x¹⁾ 5	3101-1x¹⁾ 5
	g					5	Į	5	
Design	g mg	5	5	5	5	5) (5	5
Design Weighing capacity	-	5 5,100	5 3,100	5 2,100	5 1,100	5 610) (5 6,100	5 3,100
Design Weighing capacity Readability Repeatability	mg	5 5,100 10	5 3,100 10	5 2,100 10	5 1,100 10	5 610 10) (5 6,100 100	5 3,100 100
Design Weighing capacity Readability Repeatability (standard deviation)	mg mg	5 5,100 10 10	5 3,100 10 10	5 2,100 10 10	5 1,100 10 10	5 610 10 10) (5 6,100 100 50 100	5 3,100 100 50
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of	mg mg mg	5 5,100 10 10 20	5 3,100 10 10 20	5 2,100 10 10 20	5 1,100 10 10 20	5 610 10 10 20	;	5 6,100 100 50 100 82	5 3,100 100 50 100
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of the operating range ²⁾ Optimal starting point of	mg mg mg g	5 5,100 10 10 20 12 8.2	5 3,100 10 10 20 12	5 2,100 10 10 20 12	5 1,100 10 10 20 12	5 610 10 10 20 12	;	5 6,100 100 50 100 82 82	5 3,100 100 50 100 82
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of the operating range ²⁾ Optimal starting point of the operating range ²⁾	mg mg mg g g	5 5,100 10 10 20 12 8.2	5 3,100 10 10 20 12 8.2	5 2,100 10 10 20 12 8.2	5 1,100 10 10 20 12 8.2	5 610 10 10 20 12 8.2) (5 6,100 100 50 100 82 82	5 3,100 100 50 100 82 82
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of the operating range ²⁾ Optimal starting point of the operating range ²⁾ Sensitivity drift between +10 to +30°C Typical stabilization time isoCAL Settings: - temperature change	mg mg mg g g ± ppm/K	5 5,100 10 10 20 12 8.2 2	5 3,100 10 10 20 12 8.2 2	5 2,100 10 10 20 12 8.2 2	5 1,100 10 20 12 8.2 2	5 610 10 10 20 12 8.2 2	;	5 6,100 100 50 100 82 82 2 1	5 3,100 100 50 100 82 82 2 1
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of the operating range ²⁾ Optimal starting point of the operating range ²⁾ Sensitivity drift between +10 to +30°C Typical stabilization time isoCAL Settings:	mg mg mg g g ± ppm/K s K	5 5,100 10 20 12 8.2 2 1	5 3,100 10 10 20 12 8.2 2 1 2	5 2,100 10 10 20 12 8.2 2 1 1 2	5 1,100 10 20 12 8.2 2 1 2 6	5 610 10 20 12 8.2 2 1 1 2 6		5 6,100 100 50 100 82 82 2 1	5 3,100 100 50 100 82 82 2 1
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of the operating range ²⁾ Optimal starting point of the operating range ²⁾ Sensitivity drift between +10 to +30°C Typical stabilization time isoCAL Settings: - temperature change - time interval Display result (depending	mg mg g g ± ppm/K s K	5 5,100 10 20 12 8.2 2 1 1 2 6	5 3,100 10 10 20 12 8.2 2 2 1 2 3	5 2,100 10 20 12 8.2 2 1 2 1 2 6	5 1,100 10 20 12 8.2 2 1 2 6	5 610 10 10 20 12 8.2 2 1 2 6 0.2 0.1		5 6,100 100 50 100 82 82 82 1 1 2 5 5 0.1 0.2	5 3,100 100 50 100 82 82 2 1 2 2
Design Weighing capacity Readability Repeatability (standard deviation) Linearity Typical starting point of the operating range ²⁾ Optimal starting point of the operating range ²⁾ Optimal starting point of the operating range ²⁾ Sensitivity drift between +10 to +30°C Typical stabilization time isoCAL Settings: - temperature change - time interval Display result (depending on the filter level)	mg mg g g ± ppm/K s K h s	5 5,100 10 20 12 8.2 2 1 2 1 2 6 6 0.1 0.2	5 3,100 10 20 12 8.2 2 1 2 6 0.1 0.2	5 2,100 10 10 20 12 8.2 2 1 2 1 2 6 0.1 0.2	5 1,100 10 20 12 8.2 2 1 2 6 0.1 0	5 610 10 10 20 12 8.2 2 1 2 6 0.2 0.1) () () () () () () () () () (5 6,100 100 50 100 82 82 2 1 2 2 1 2 5 0.1 0.2 2 180	5 3,100 100 50 100 82 82 2 1 2 1 2 6 0.1 0.2

Verified Models with Country-specific Type Approval Certificate

Model		26-1x ²⁾	225D-1x ²⁾	125-1x ²⁾	324-1x ²⁾
Design		1	2	2	2
Accuracy class					I
Type ³⁾		SQP-H	SQP-F	SQP-F	SQP-G
Max	g	21	120 220	120	320
Scale interval d	g	0.000002	0.00001 0.0001	0.00001	0.0001
Verification scale interval e	g	0.001	0.001	0.001	0.001
Min	g	0.001	0.001	0.001	0.01
Min (only for Models10IN)	g	0.1	0.1	0.1	0.1
Tare equalization range (subtractive)		<100 % of the ma	x. weighing capacity		
Typical starting point of the operating range 4)	g	0.004	0.025**	0.025**	0.160
Optimal starting point of the operating range 4)	g	0.00164*	0.0082**	0.0082**	0.082
Typical stabilization time	S	8	6 2	6	2
isoCAL:					
– Temperature change	K	1.5	1.5	1.5	1.5
– Time interval	h	4	4	4	4
Display result (depending on the set filter level)	S	0.2 0.4	0.2 0.4	0.2 0.4	0.2 0.2
Weighing pan size	mm	Ø 50	Ø 80 (optional Ø 90)	arnothing 80 (optional $arnothing$ 90)	Ø 90
Weighing chamber height***	mm	218	218	218	218
Net weight, approx.	kg	8.0	7.8	7.8	7.9
IP protection class		IP43	IP43	IP43	IP43

* In combination with glass draft shield YHK01SQP

In combination with weighing pan, 80 mm, slotted YSP01SQP

*** Upper edge of the weighing pan to the lower edge of the upper draft shield panel

²⁾ Possible terms for country-specific models:

x = CEU: Verified balances with EC Type Approval Certificate D12-09-014 (for EU except France, Italy, and Switzerland)

x = CFR: Verified balances with EC Type Approval Certificate D12-09-014 for France only

x = CIT: Verified balances with EC Type Approval Certificate D12-09-014 for Italy only x = CCH: Verified balances with EC Type Approval Certificate D12-09-014 for Switzerland only

x = CN: CMC Type Approval Certificate for China

x = OJP: Balance with Type Approval Certificate for Japan

x = OBR: Balance with Type Approval Certificate for Brazil

x = ORU: Balance with Type Approval Certificate for Russia

x = OIN: Balance with Type Approval Certificate for India

x = OAU: Balance with Type Approval Certificate for Australia

³⁾ All models with "...CN": type "SQP"

⁴⁾ According to USP (United States Pharmacopeia) Chapter 41, the optimal operating range is defined from 820d to maximum weighing capacity. Depending on the installation location and environmental conditions, the value could be higher.

Model		224-1x ²⁾	124-1x ^{2]}	1103-	1 x ²⁾	613- 1	x ²⁾	513	-1x ²⁾	31	3-1x ²⁾	213-1x ²⁾
Design		3	3	4		4		4		4		4
Accuracy class		I		I		(\mathbb{I})				I)	
Type ³⁾		SQP-A	SQP-A	SQP-I		SQP-B		SQP-	-B	_		SQP-B
Max	g	220	120	1,100		610		510		31		210
Scale interval d	mg	0.1	0.1	1		1		1		1		1
Verification scale interval e	mg	1	1	10		10		10		10		10
Min	mg	10	10	100		20		20		20		20
Min (only for Models10IN)	mg	100	100	1,000		200		200		20	0	200
Tare (subtractive)		< 100% of	max. weighi	ng capacity								
Typical starting point of the operating range ⁴⁾	g	0.12	0.12	1.5		1.5		1.5		1.5		1.5
Optimal starting point of the operating range ⁴⁾	g	0.082	0.082	0.82		0.82		0.82		0.8	32	0.82
Typical stabilization time	S	2	2	1.5		1		1		1		1
isoCAL:												
 Temperature change Time interval 	K h	1.5 4	1.5 4	1.5 4		2 6		2 6		2 6		2 6
Display result (depending on the set filter level)	S	0.2	0.2	0.1 0.2	2	0.1 0.	.2	0.1	0.2	0.1	0.2	0.1 0.2
Weighing pan size	mm	Ø 90	Ø 90	Ø 120		Ø 120)	Ø 12	20	Ø	120	Ø 120
Weighing chamber height***	mm	209	209	209		209		209		20	9	209
Net weight, approx.	kg	5.1	5.1	5.9		5.1		5.1		5.1		5.1
Model		$6102 - 1x^{2}$	5102-1x ²⁾	3102-1x ²⁾	210	2_1x ²⁾	1102-	1 x ²⁾	612 - 1x	2)	$6101 - 1x^2$	⁾ 3101-1x ²
Design		5	5	5	5	- 17	5	17	5	•	5	5
Accuracy class												
Type ³⁾		SQP-C	SQP-C	SQP-C	SQP	-C	SQP-C		SQP-C		SQP-C	SQP-C
Max	g	6,100	5,100	3,100	2,10		1,100		610		6,100	3,100
Scale interval d	mg	10	10	10	10		10		10		100	100
Verification scale interval e	mg	100	100	100	100		100		100		100	100
Min	mg	500	500	500	500		500		500		5,000	5,000
Min (only for Models10IN)	g	5	5	5	5		5		5		5	5
Tare (subtractive)		< 100% of	max. weighi	ng capacity								
Typical starting point of the operating range ⁴⁾	g	12	12	12	12		12		12		82	82
Optimal starting point of the operating range 4)	g	8.2	8.2	8.2	8.2		8.2		8.2		82	82
Typical stabilization time isoCAL:	S	1	1	1	1		1		1		1	1
 Temperature change Time interval 	K h	2 6	2 6	2 6	2 6		2 6		2 6		2 6	2 6
Display result (depending on the set filter level)	S	0.1 0.2	0.1 0.2	0.1 0.2	0.1	0.2	0.1 0.2	2	0.1 0.2		0.1 0.2	0.1 0.2
Weighing pan size	mm	Ø 180	Ø 180	Ø180	Ø 1	80	Ø 180		Ø 180		Ø 180	Ø 180
Net weight, approx.	kg	5.2	5.2	5.2	5.2		5.2		5.2		5.2	5.2


Optional Accessories

Printers and Communications	
Premium GLP Laboratory Printer	YDP30
 Printer paper for GLP laboratory printer Endless labels for GLP laboratory printer 	69Y03285 69Y03286
	YDP40
Standard Laboratory Printer – Printer paper for standard laboratory printer	69Y03287
Data communication cable, USB USB A	YCC04-D09
Data communication cable, mini USB RS232, 9-pin	YCC03-D09
Data communication cable, mini USB RS232, 25-pin	YCC03-D25
General	
Battery Pack for Standard Lab Balances	YRB11Z
Draft shield for balances with a readability of 10 mg	YDS01SQP
Round glass draft shield for balances with a readability of 1 mg	YDS02SQP
Glass draft shield for balances with a readability of 0.002 mg,	YHK01SQP
for increasing the weighing performance	
In-use cover for balances with a readability of 0.01 mg 0.002 mg	6960SE05
In-use cover for balances with a readability of 0.1 mg 1 mg	6960SE01
In-use cover for balances with a readability of 10 mg	6960SE02
Dust cover for balances with a readability of 0.1 mg $ $ 1 mg	6960SE03
Dust cover for balances with a readability of 0.01 mg 0.002 mg	6960SE04
Certificate of USP minimum weight	84CGNA
Weighing Pans (for balances design 1)	
Weighing pan, diameter 80 mm, slotted, for increasing the weighing performance	YSP01SQP
Weighing pan, diameter 90 mm; includes conversion kit	YWP01SQP
Filter weighing pan, diameter 130 mm	YFW01SQP
Stainless steel weighing pan set, diameter 50 mm, for balances with a readability of 0.002 mg	VF4589
Density Determination	
Density kit for balances with a readability of 0.01 mg	VF4601
Density kit for balances with a readability of 0.1 mg $ $ 1 mg	YDK03
Density kit for balances with a readability of 10 mg	YDK04


Calibration Weights	
Calibration weight for lab balance model 26 – Proof Line knob weight 20 g, OIML class E2, with DAkkS certificate	YCW422-AC-02
Calibration weight for lab balance model 324; 224; 313; 213 – Proof Line knob weight 200 g, OIML class E2, with DAkkS certificate	YCW522-AC-02
Calibration weight for lab balance model 225D; 125; 124 – Proof Line knob weight 100 g, OIML class E2, with DAkkS certificate	YCW512-AC-02
Calibration weight for lab balance model 613; 513; 612 – Proof Line knob weight 500 g, OIML class E2, with DAkkS certificate	YCW552-AC-02
Calibration weight for lab balance model 6102; 5102 – Proof Line knob weight 5 kg, OIML class E2, with DAkkS certificate	YCW652-AC-02
Calibration weight for lab balance model 3102; 2102 – Proof Line knob weight 2 kg, OIML class E2, with DAkkS certificate	YCW622-AC-02
Calibration weight for lab balance model 1103; 1102 – Proof Line knob weight 1 kg, OIML class E2, with DAkkS certificate	YCW612-AC-02
Calibration weight for lab balance model 6101 – Proof Line knob weight 5 kg, OIML class F1, with DAkkS certificate	YCW653-AC-02
Calibration weight for lab balance model 3101 – Proof Line knob weight 2 kg, OIML class F2, with DAkkS certificate	YCW624-AC-02

Technical Drawings


Models with a readability of 0.002 mg, in mm

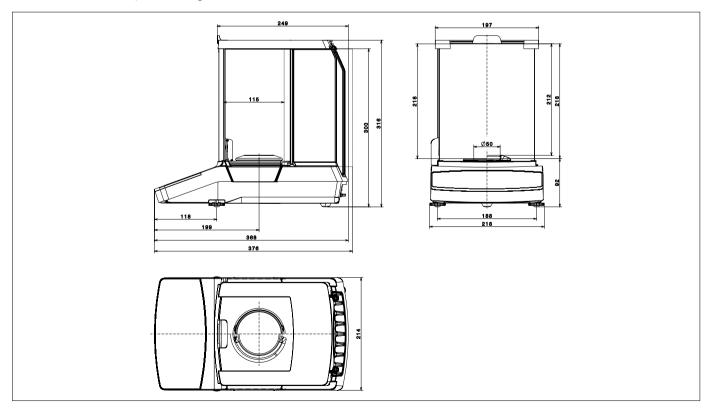


Models with a readability of 0.01 mg and 324-1x, in mm

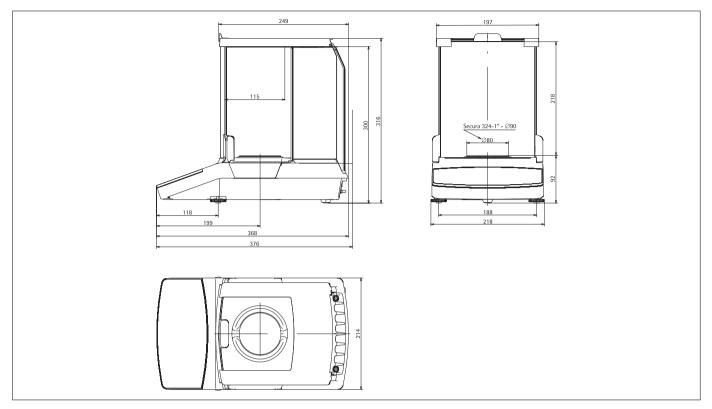


Models with a readability of 0.1 mg (except 324-1x), in mm

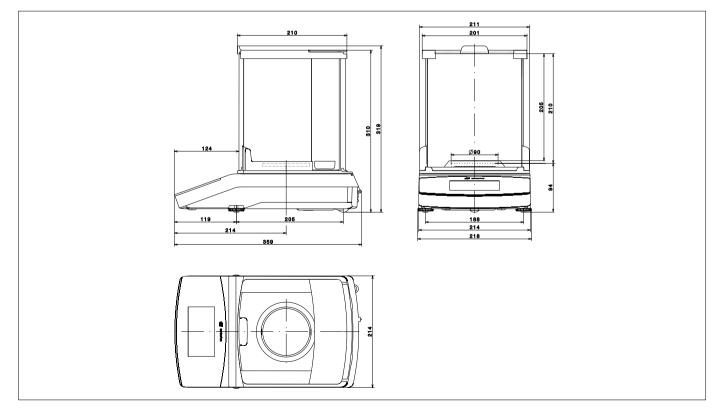

Models with a readability of 1 mg, in mm

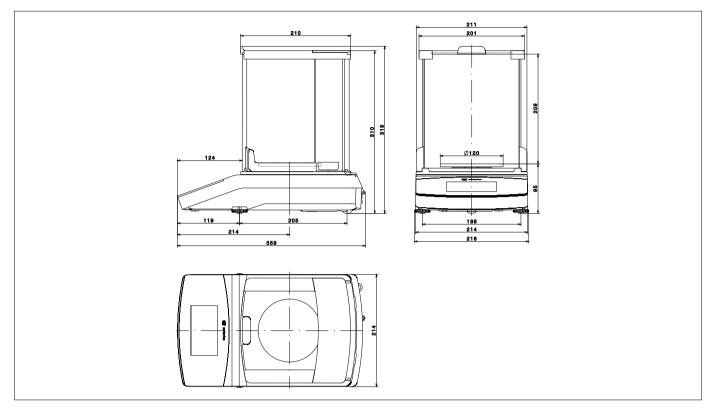

Models with a readability of \geq 10 mg, in mm

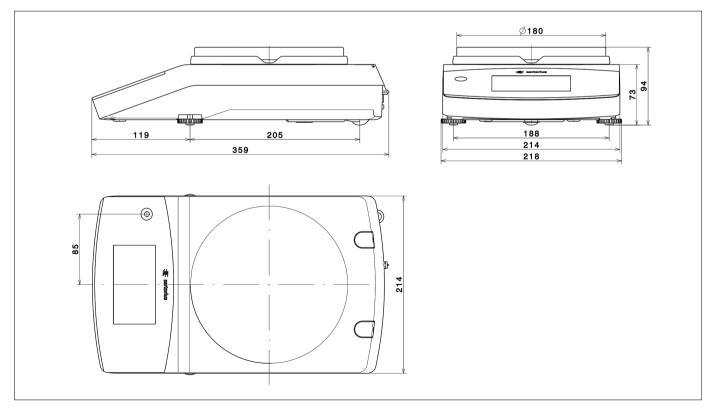



Pricing on any accessories shown can be found by keying the part number into the search box on our website. The specifications listed in this brochure are subject to change by the manufacturer and therefore cannot be guaranteed to be correct. If there are aspects of the specification that must be guaranteed, please provide these to our sales team so that details can be confirmed.

www.wolflabs.co.uk

Tel : 01759 301142 Fax : 01759 301143 sales@wolflabs.co.uk

Please contact us if this literature doesn't answer all your questions.